
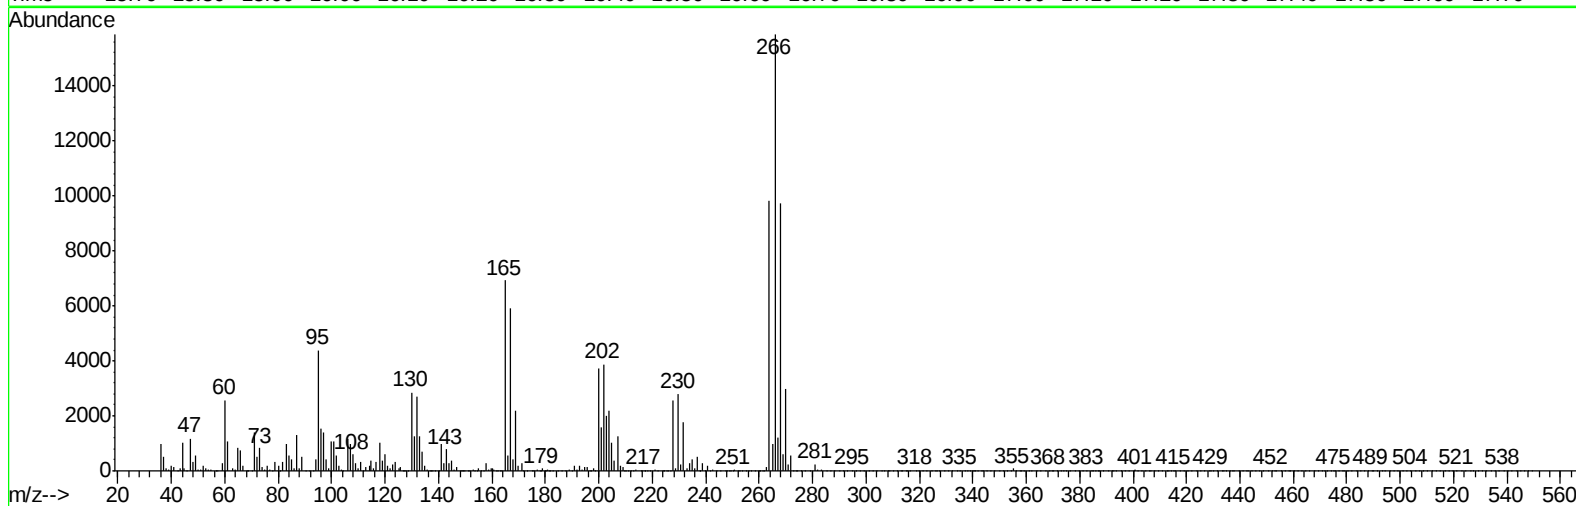


Data File : BP001545.D
Acq On : 08 Jan 2020 09:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 05:52:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 15:02:19 2020
Response via : Initial Calibration

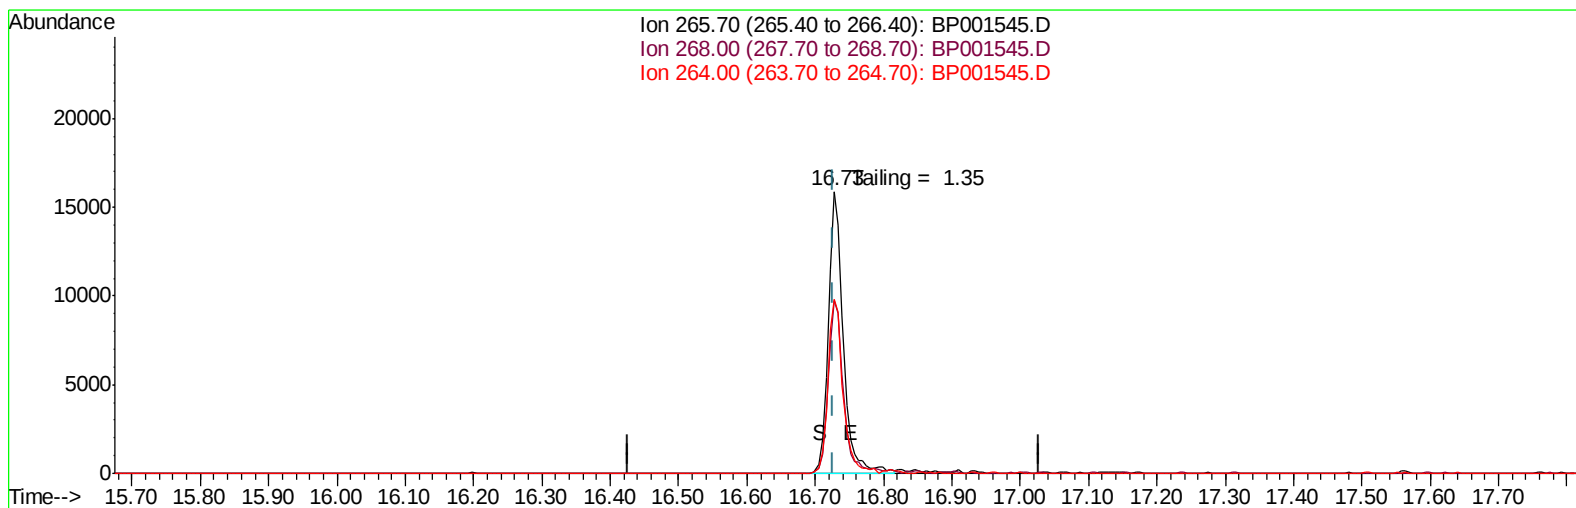

TIC: BP001545.D

(70) Pentachlorophenol (C)



16.728min (+0.000) 370492.55ng

response 24136

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	61.25
264.00	63.60	61.88
0.00	0.00	0.00

Data File : BP001545.D
Acq On : 08 Jan 2020 09:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 05:52:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 15:02:19 2020
Response via : Initial Calibration

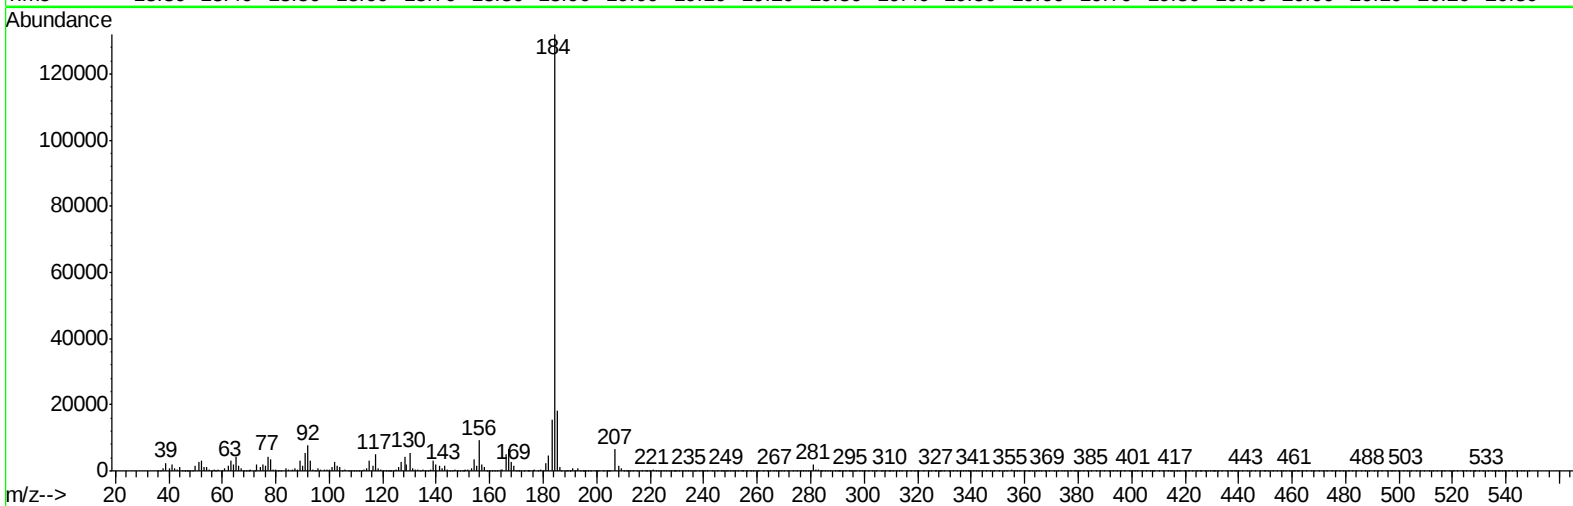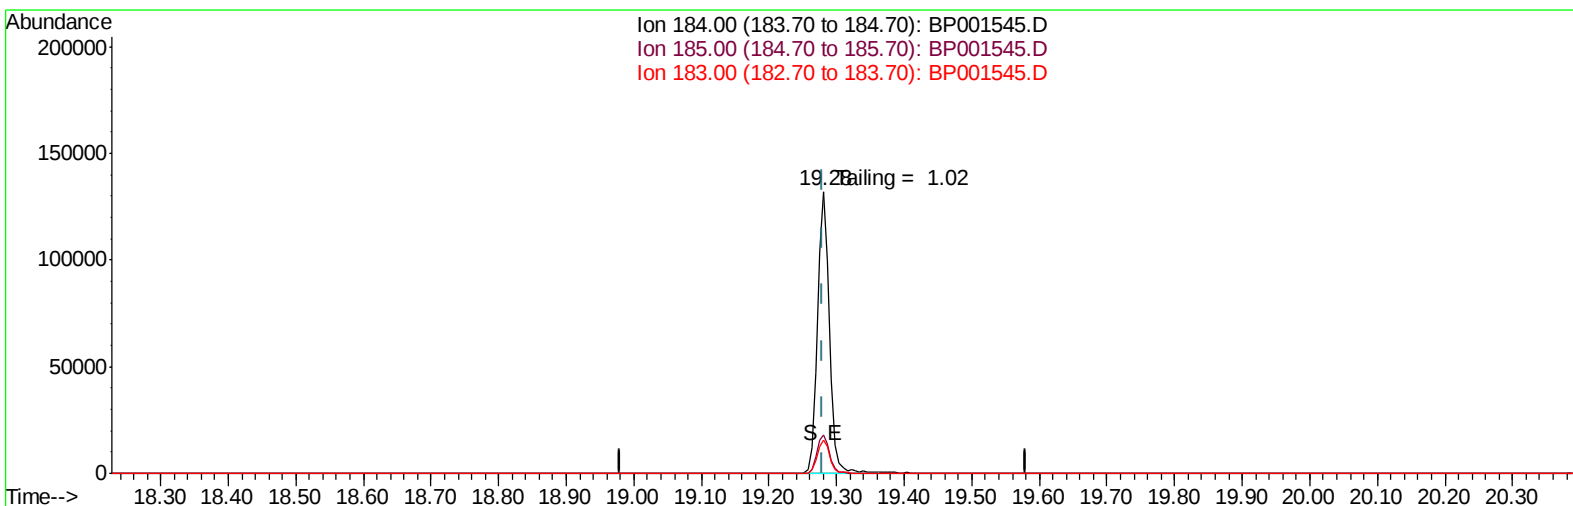

TIC: BP001545.D

(77) Benzidine

19.281min (+0.000) 520853.06ng

response 166501

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	13.69
183.00	11.70	11.75
0.00	0.00	0.00