
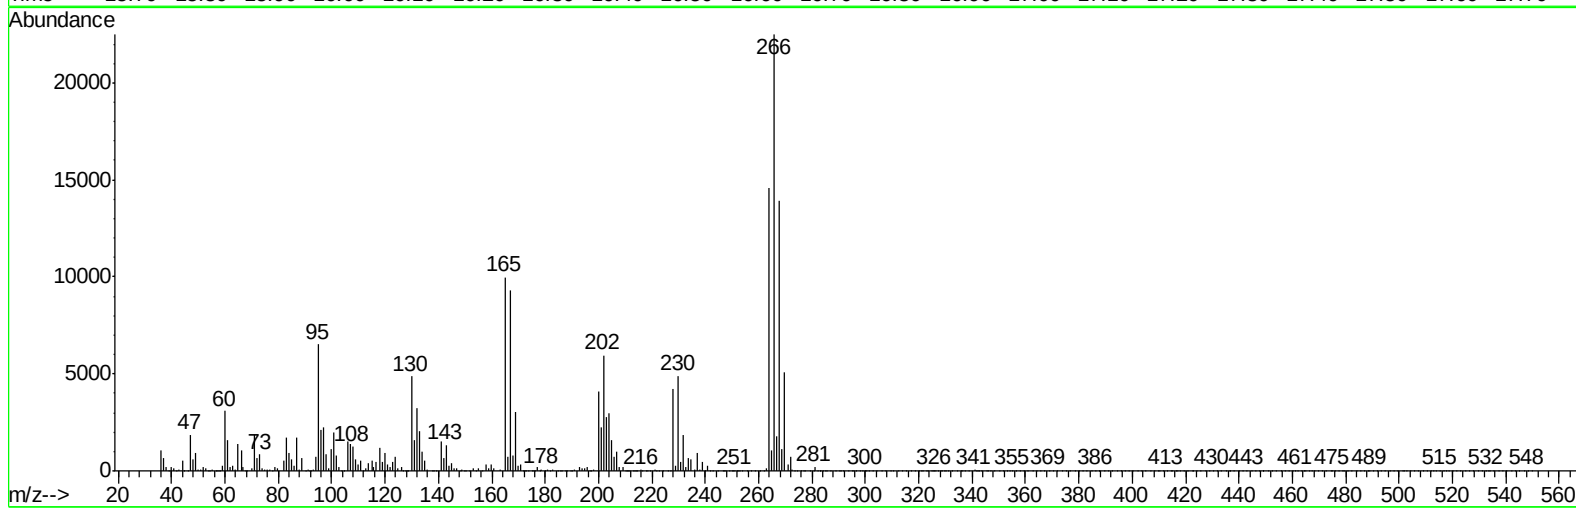


Data File : BP001555.D
Acq On : 08 Jan 2020 16:56
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 05:53:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 15:02:19 2020
Response via : Initial Calibration

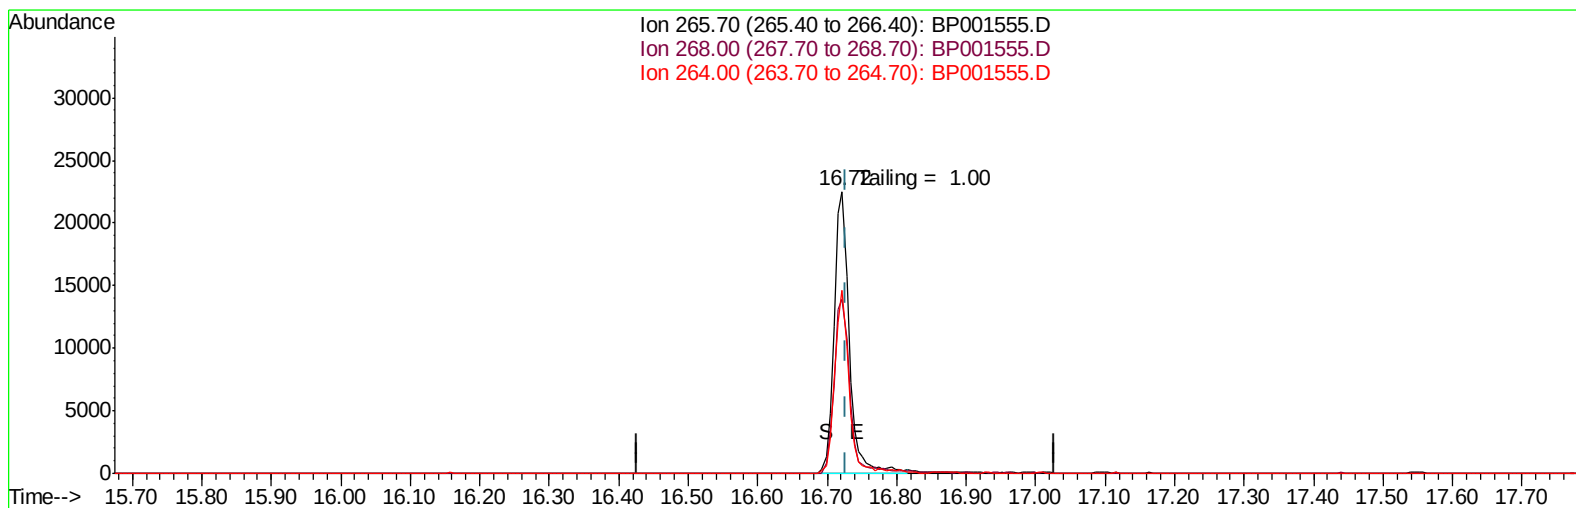

TIC: BP001555.D

(70) Pentachlorophenol (C)



16.722min (-0.006) 56420.53ng

response 33080

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	61.84
264.00	63.60	64.79
0.00	0.00	0.00

Data File : BP001555.D
Acq On : 08 Jan 2020 16:56
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 05:53:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 15:02:19 2020
Response via : Initial Calibration

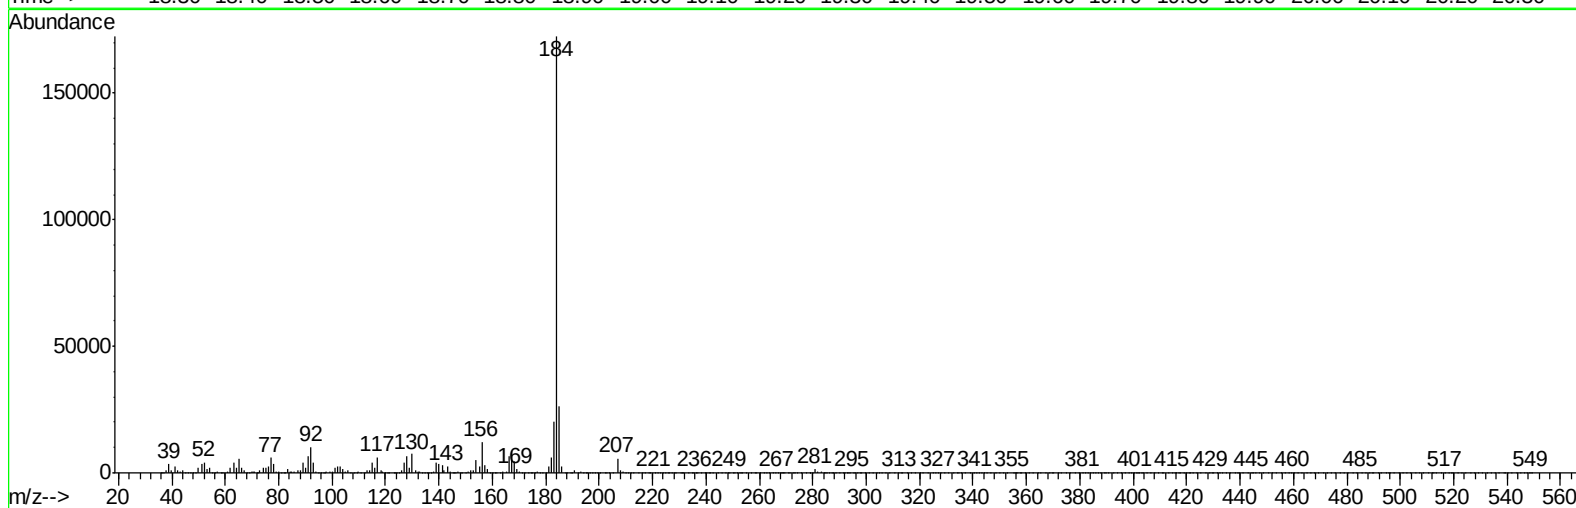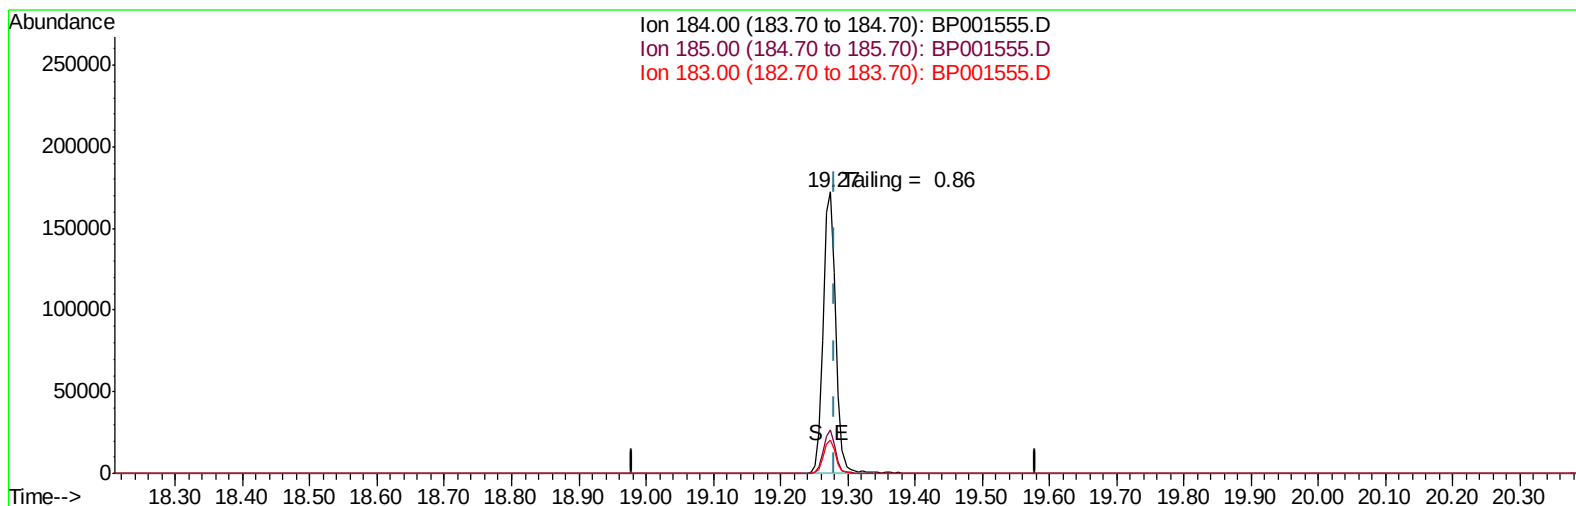

TIC: BP001555.D

(77) Benzidine

19.274min (-0.006) 47006.91ng

response 227547

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	15.37
183.00	11.70	11.62
0.00	0.00	0.00