


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP010820\
 Data File : BP001545.D
 Acq On : 08 Jan 2020 09:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 15:02:19 2020

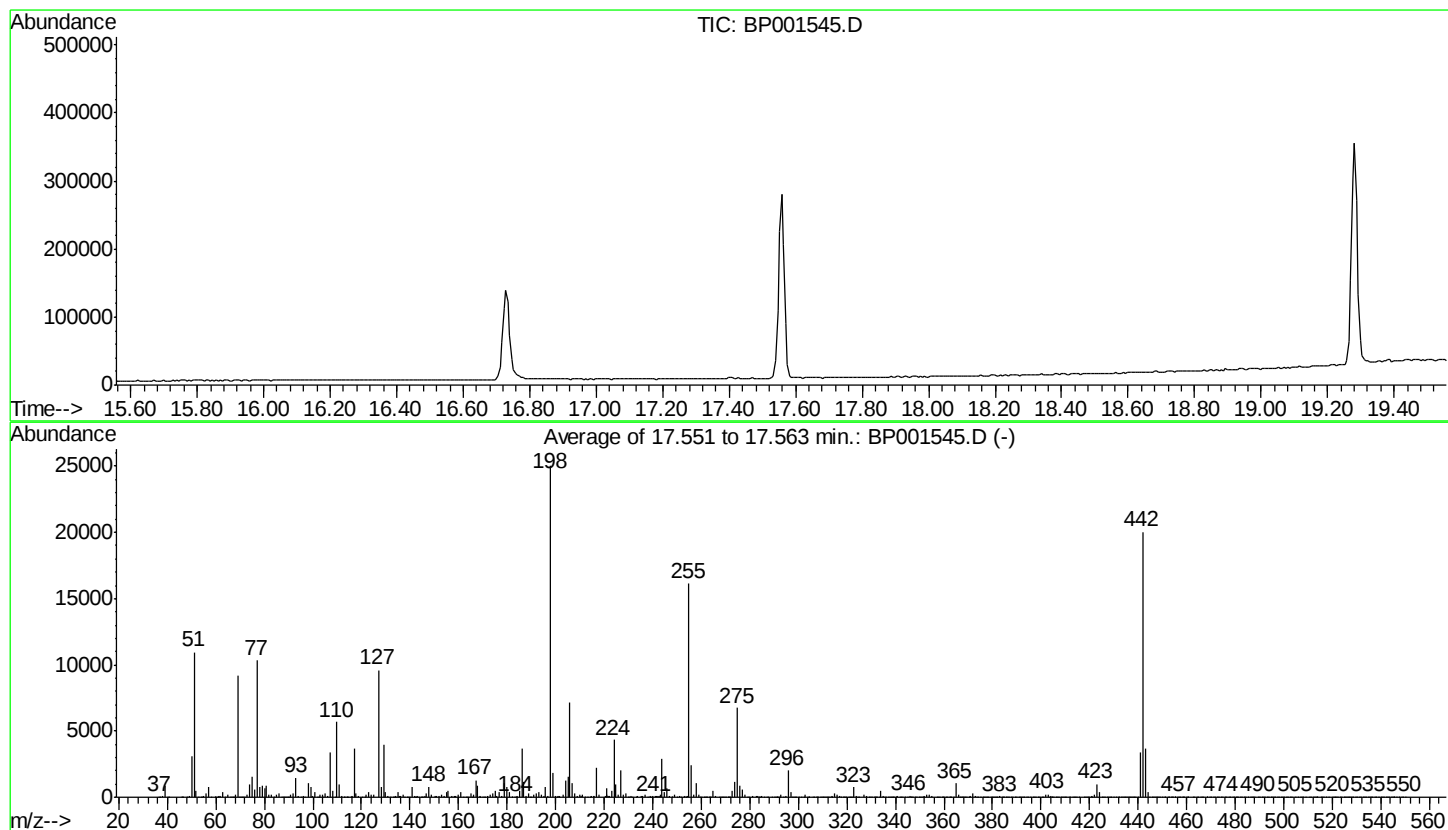

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	10967	PASS
68	69	0.00	2	1.9	177	PASS
69	198	0.00	100	36.6	9165	PASS
70	69	0.00	2	0.3	30	PASS
127	198	10	80	38.4	9603	PASS
197	198	0.00	2	0.5	120	PASS
198	198	100	100	100.0	25040	PASS
199	198	5	9	7.5	1886	PASS
275	198	10	60	27.0	6750	PASS
365	198	1	100	4.2	1049	PASS
441	198	0.01	100	13.4	3353	PASS
442	198	50	100	80.1	20051	PASS
443	442	15	24	18.1	3634	PASS