


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP010820\
 Data File : BP001555.D
 Acq On : 08 Jan 2020 16:56
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 15:02:19 2020

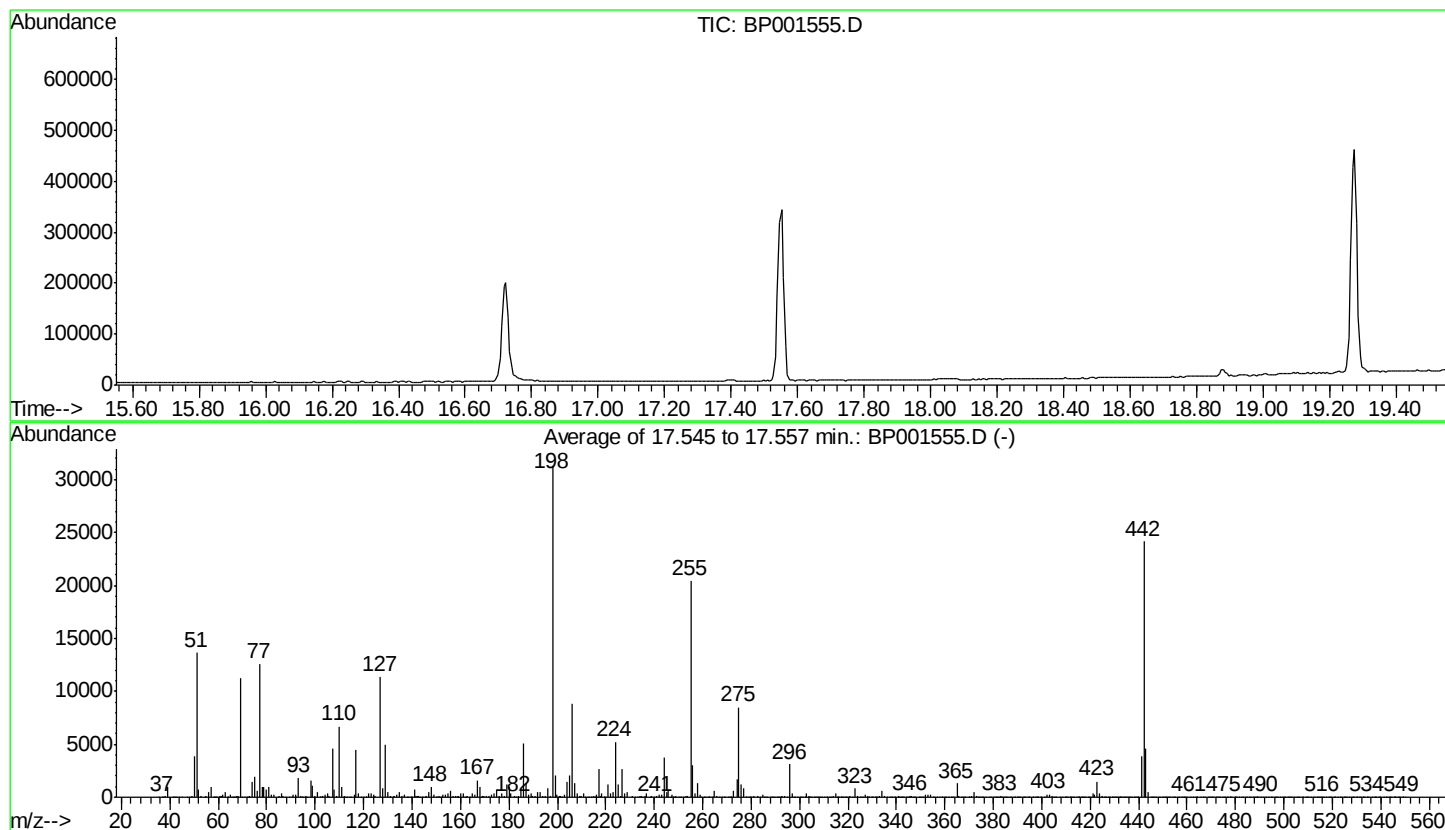

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	13613	PASS
68	69	0.00	2	1.0	113	PASS
69	198	0.00	100	35.9	11240	PASS
70	69	0.00	2	0.6	64	PASS
127	198	10	80	36.3	11374	PASS
197	198	0.00	2	0.4	131	PASS
198	198	100	100	100.0	31312	PASS
199	198	5	9	6.4	2009	PASS
275	198	10	60	27.1	8498	PASS
365	198	1	100	4.1	1282	PASS
441	198	0.01	100	12.3	3860	PASS
442	198	50	100	77.1	24146	PASS
443	442	15	24	19.2	4632	PASS