
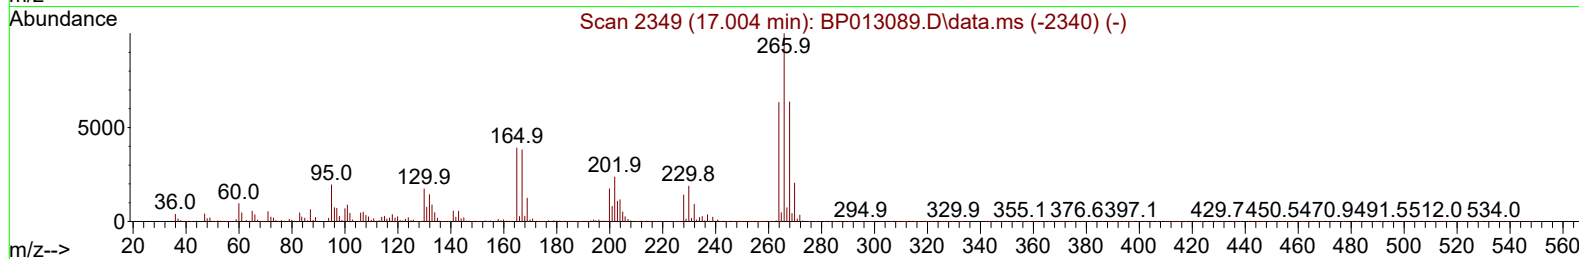
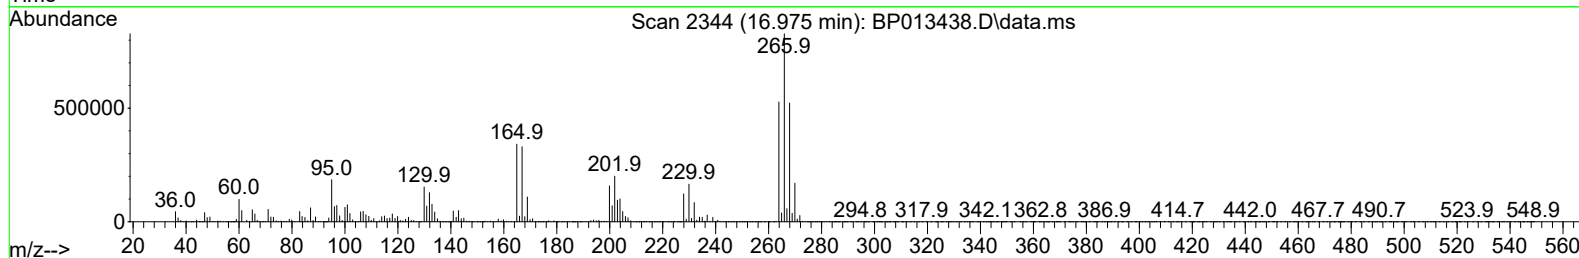


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013438.D
Acq On : 11 Jan 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 05:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 02:16:32 2023
Response via : Initial Calibration

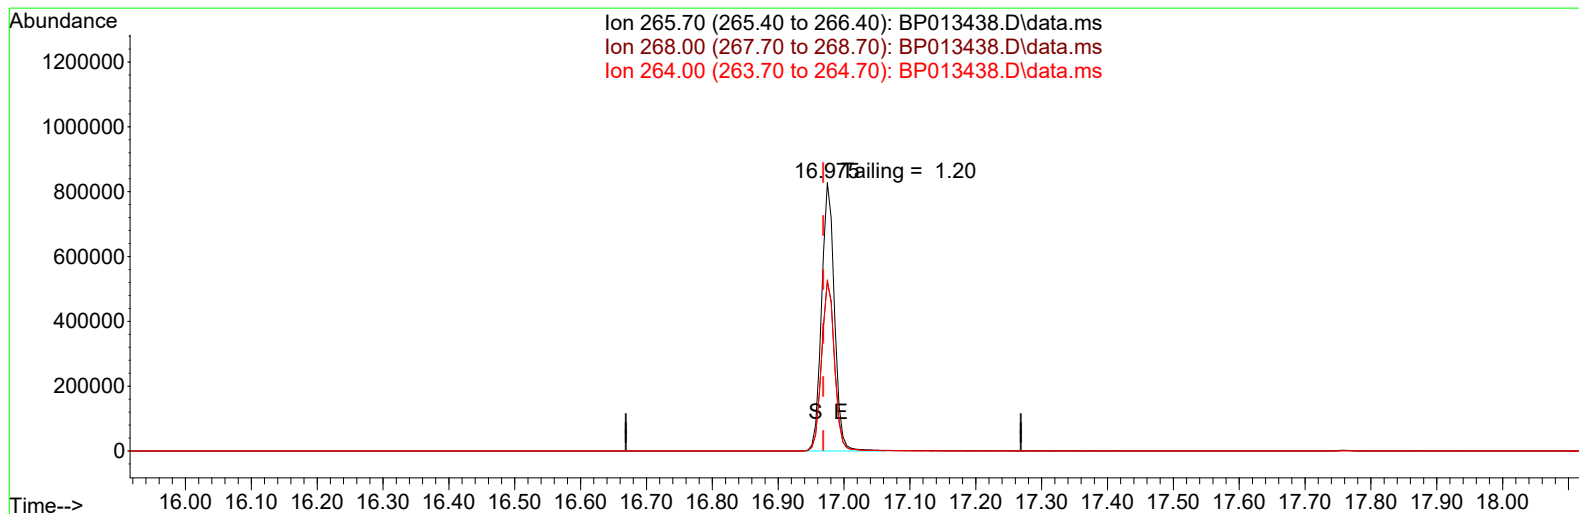

TIC: BP013438.D\data.ms

(70) Pentachlorophenol (C)




16.975min (+ 0.006) 79715.29 ng

response 1128989

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.16
264.00	63.30	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
 Data File : BP013438.D
 Acq On : 11 Jan 2023 11:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 05:00:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 02:16:32 2023
 Response via : Initial Calibration

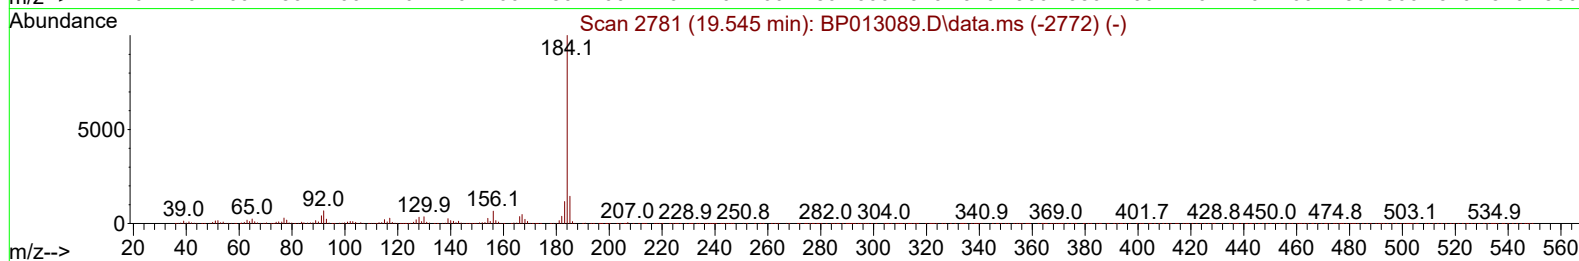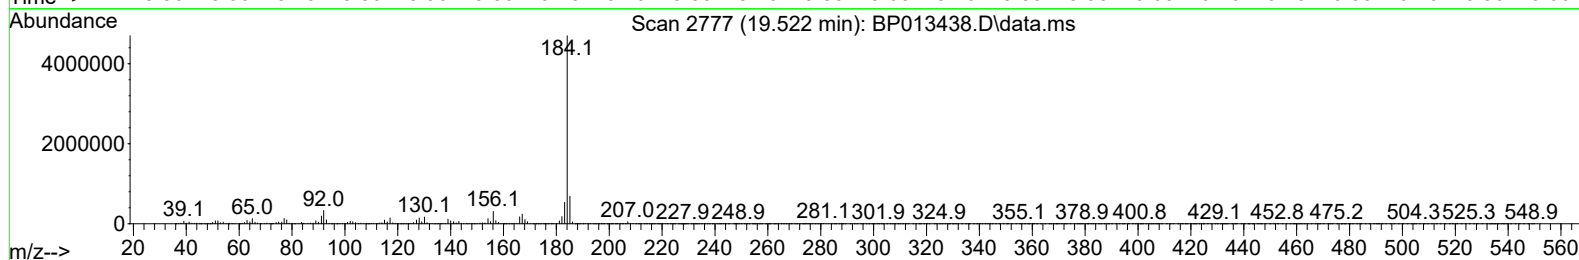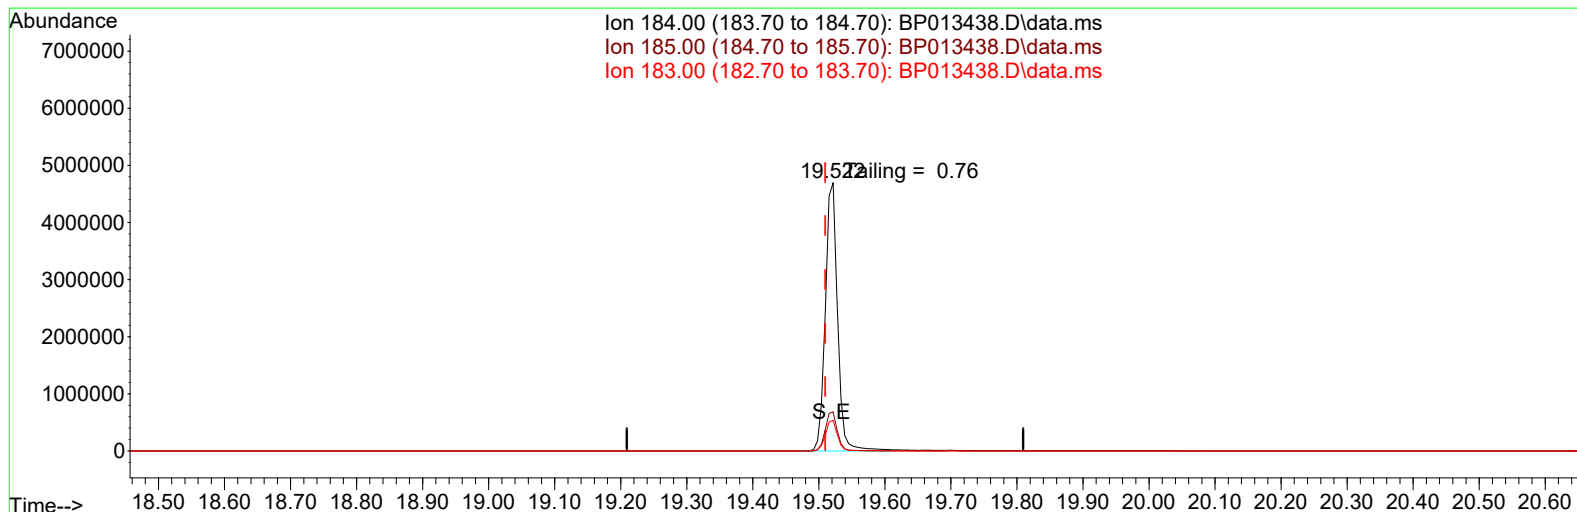

TIC: BP013438.D\data.ms

(77) Benzidine**19.522min (+ 0.012) 11344.45 ng****response 6072148**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.60
183.00	11.70	11.44
0.00	0.00	0.00