

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
 Data File : BP013440.D
 Acq On : 11 Jan 2023 12:54
 Operator : CG/JU
 Sample : PB150163BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150163BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.005	304	309	320	rBV	1405596	2012825	8.00%	1.532%
2	5.475	382	389	398	rBV	10448130	15185135	60.32%	11.560%
3	7.081	654	662	678	rBV	9879271	15332499	60.90%	11.673%
4	7.916	797	804	812	rBV	1985746	3108098	12.35%	2.366%
5	9.087	994	1003	1017	rBV	5764235	9511400	37.78%	7.241%
6	10.722	1272	1281	1291	rBV	2395713	4093146	16.26%	3.116%
7	13.181	1691	1699	1714	rBV	13992745	20792183	82.59%	15.829%
8	14.557	1926	1933	1942	rBV	3515181	5016872	19.93%	3.819%
9	16.051	2179	2187	2207	rBV	10314193	14467159	57.47%	11.014%
10	17.316	2396	2402	2413	rBV	3865398	5501764	21.85%	4.188%
11	19.563	2781	2784	2789	rBV	255533	292009	1.16%	0.222%
12	19.875	2831	2837	2848	rBV	19987934	25175510	100.00%	19.166%
13	20.581	2954	2957	2961	rBV	244756	303493	1.21%	0.231%
14	21.404	3092	3097	3107	rBV	3946776	5384740	21.39%	4.099%
15	23.863	3509	3515	3530	rVB	2560526	5178114	20.57%	3.942%




Sum of corrected areas: 131354947

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013440.D
Acq On : 11 Jan 2023 12:54
Operator : CG/JU
Sample : PB150163BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150163BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

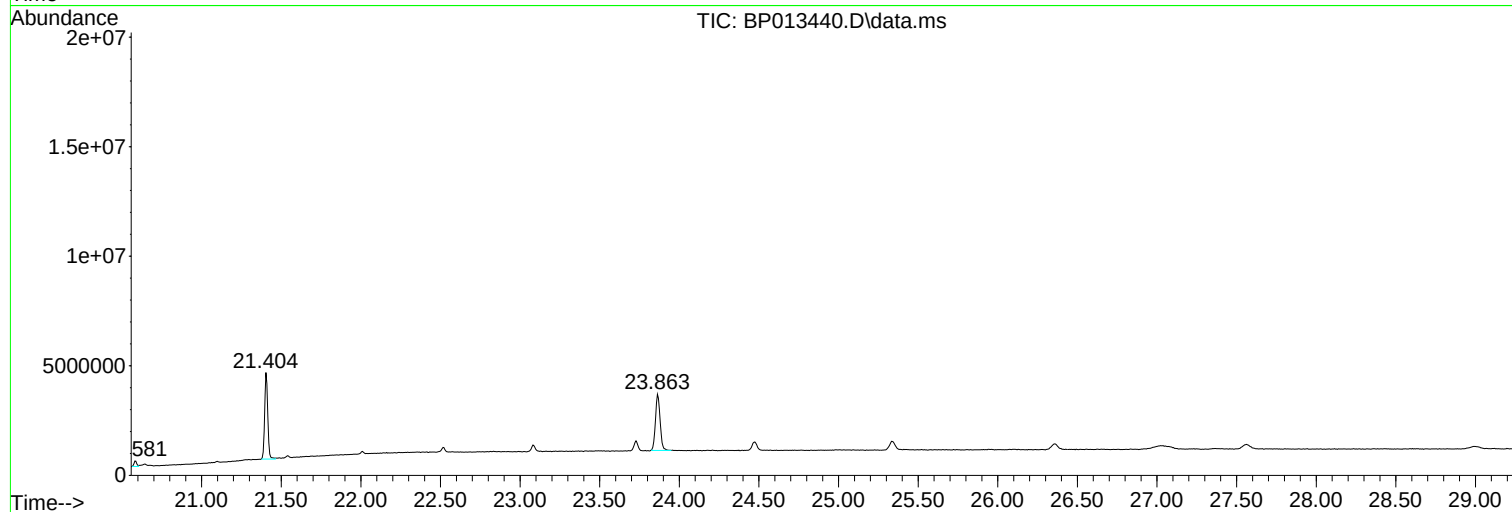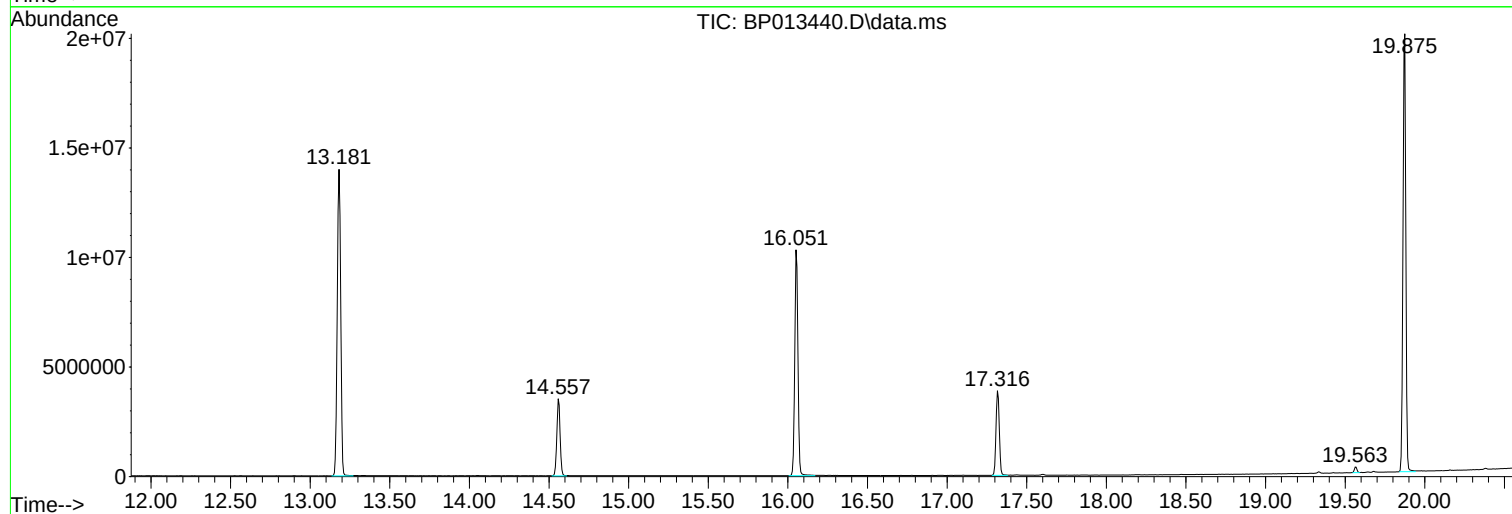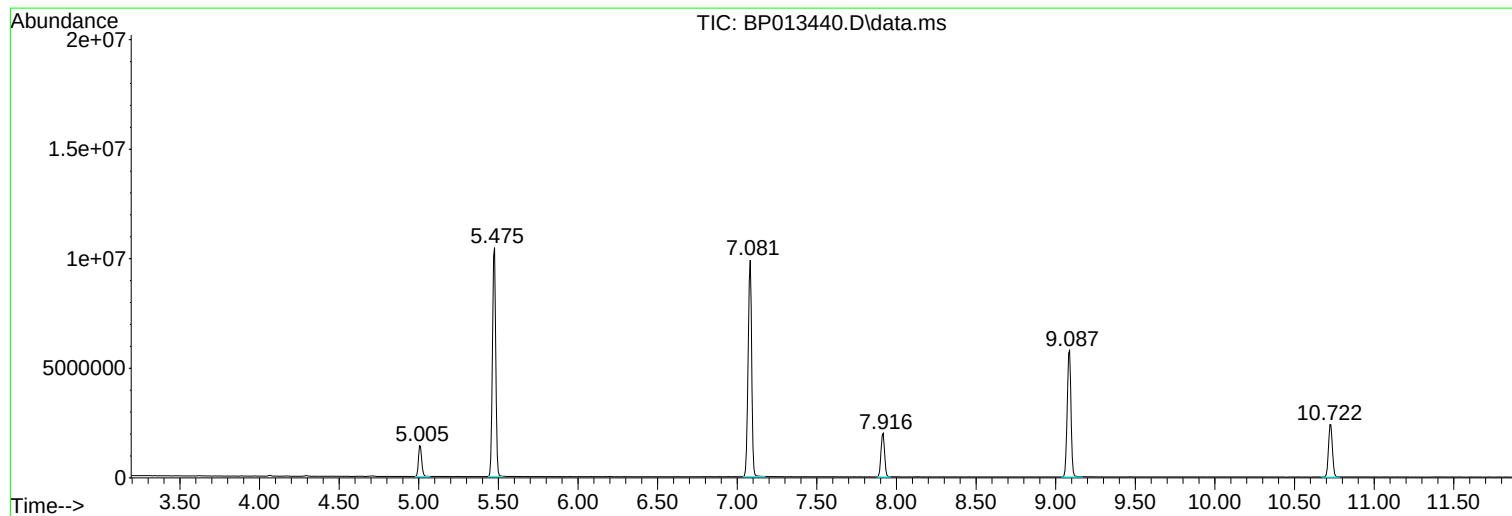

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013440.D
Acq On : 11 Jan 2023 12:54
Operator : CG/JU
Sample : PB150163BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
PB150163BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.005	12.95 ng	2012830	1,4-Dichlorobenzene-d4			7.916
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	Acetic acid, 1,1-dimethylethyl e...		116	C6H12O2	000540-88-5	32
3	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	25
4	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	12
5	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9

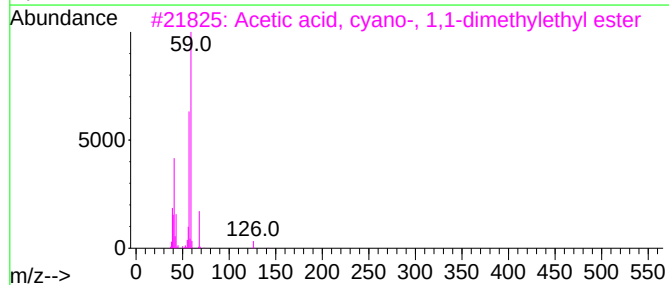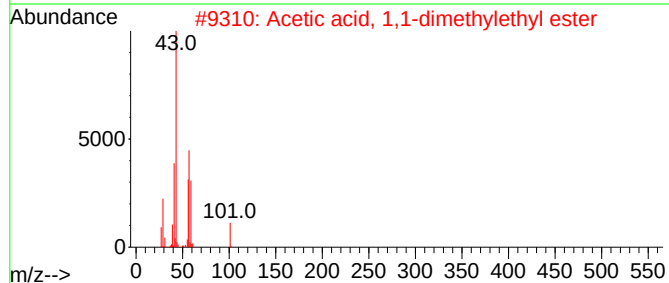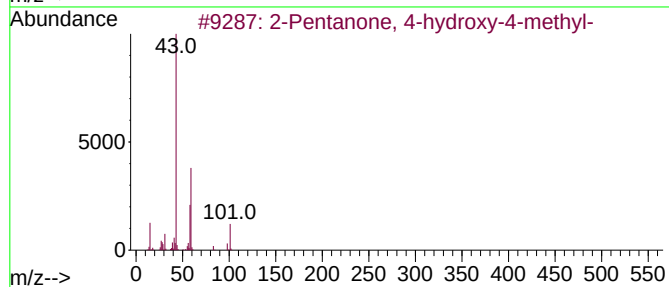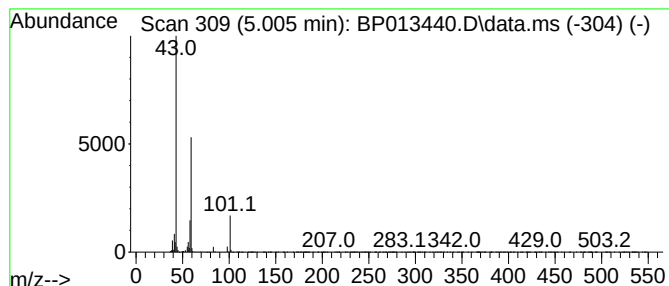

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013440.D
Acq On : 11 Jan 2023 12:54
Operator : CG/JU
Sample : PB150163BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150163BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.005	12.9	ng	2012830	1	7.916	3108100	20.0