

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
 Data File : BP013442.D
 Acq On : 11 Jan 2023 14:12
 Operator : CG/JU
 Sample : 01051-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 72-11933

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.011	300	310	317	rVB2	302896	552743	1.68%	0.217%
2	5.475	381	389	404	rVB	9455923	14249955	43.35%	5.583%
3	5.958	466	471	488	rVB4	232391	666830	2.03%	0.261%
4	7.087	655	663	675	rVB	9343032	15110796	45.96%	5.921%
5	7.917	796	804	811	rVB	2639495	4268341	12.98%	1.672%
6	8.522	901	907	912	rBV	405598	697919	2.12%	0.273%
7	9.087	995	1003	1009	rBV	5883209	9581230	29.14%	3.754%
8	9.193	1009	1021	1026	rBV7	227928	757788	2.31%	0.297%
9	9.363	1042	1050	1054	rBV6	256017	722406	2.20%	0.283%
10	9.440	1055	1063	1067	rBV3	562342	1248498	3.80%	0.489%
11	9.987	1150	1156	1167	rBV	454713	1361821	4.14%	0.534%
12	10.316	1206	1212	1215	rBV4	432579	943157	2.87%	0.370%
13	10.728	1276	1282	1292	rVB	3399220	5659254	17.21%	2.217%
14	13.187	1694	1700	1709	rVB	13017395	21279054	64.73%	8.337%
15	13.340	1722	1726	1729	rBV	2446784	3960534	12.05%	1.552%
16	13.981	1831	1835	1843	rBV	9274765	17164932	52.21%	6.725%
17	14.393	1901	1905	1913	rVB	10386690	19800597	60.23%	7.758%
18	21.557	3119	3123	3128	rVB	19629232	31510821	95.85%	12.346%
19	22.086	3210	3213	3218	rVB2	8050590	10387147	31.60%	4.070%
20	22.627	3300	3305	3318	rVB	12567572	32874697	100.00%	12.881%
21	23.533	3453	3459	3475	rVB	11471521	32492786	98.84%	12.731%
22	23.880	3514	3518	3524	rVB2	3335114	5705609	17.36%	2.236%
23	24.610	3635	3642	3652	rVB2	7293998	24229034	73.70%	9.493%




Sum of corrected areas: 255225949

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013442.D
Acq On : 11 Jan 2023 14:12
Operator : CG/JU
Sample : 01051-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11933

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

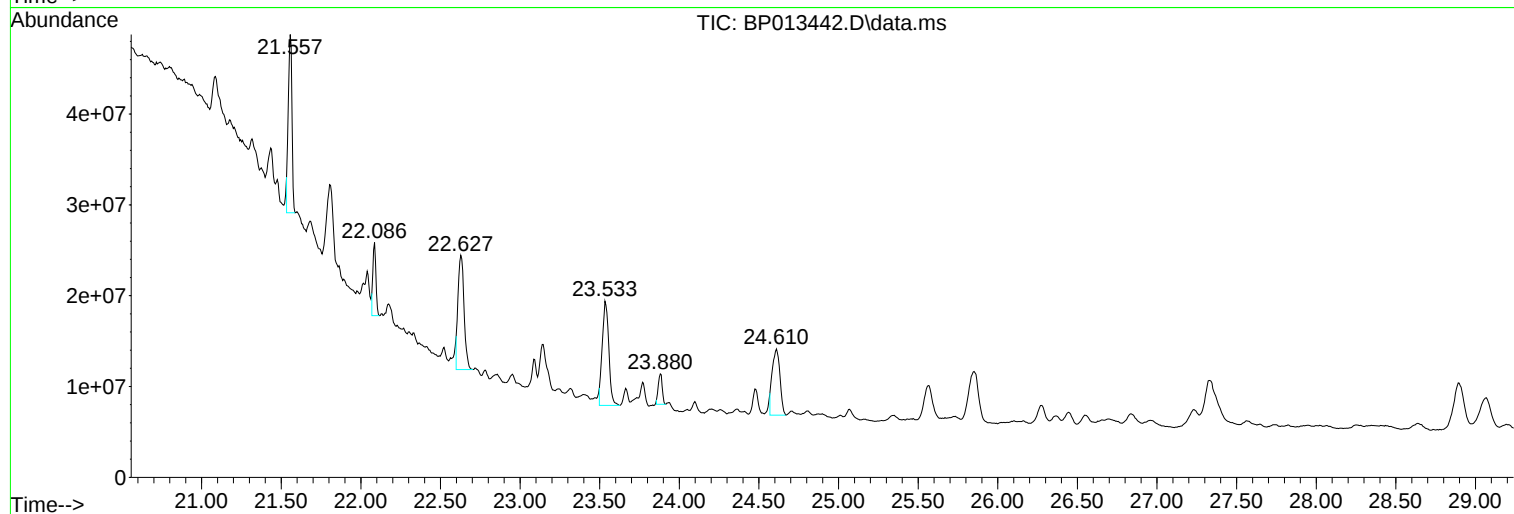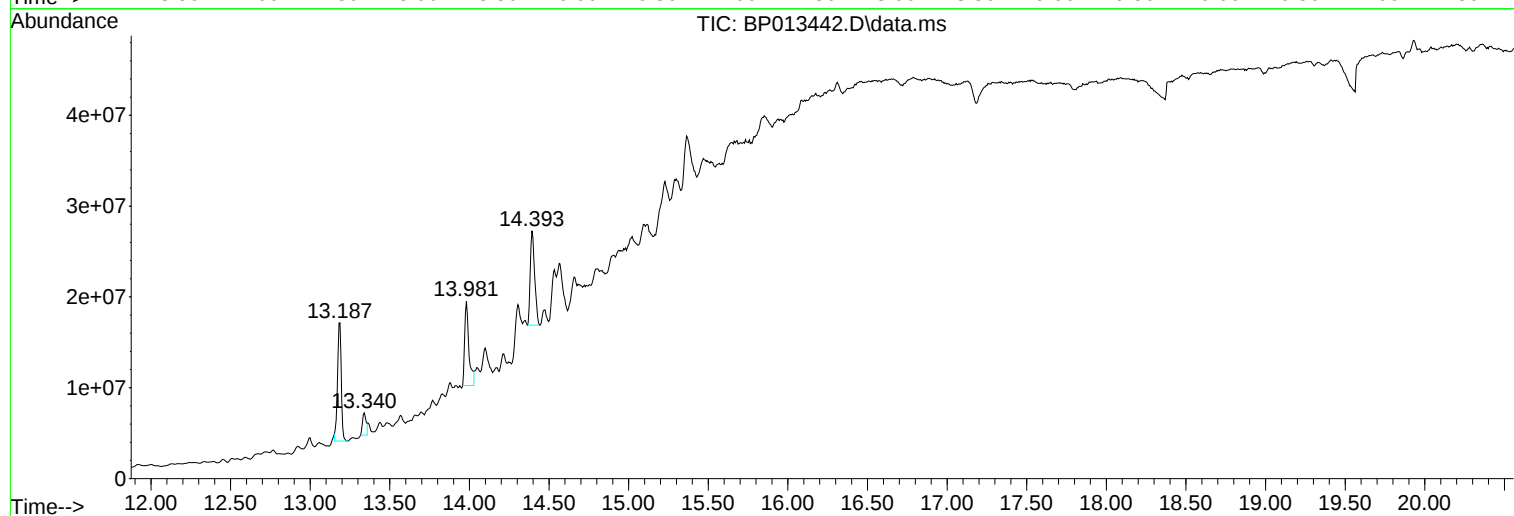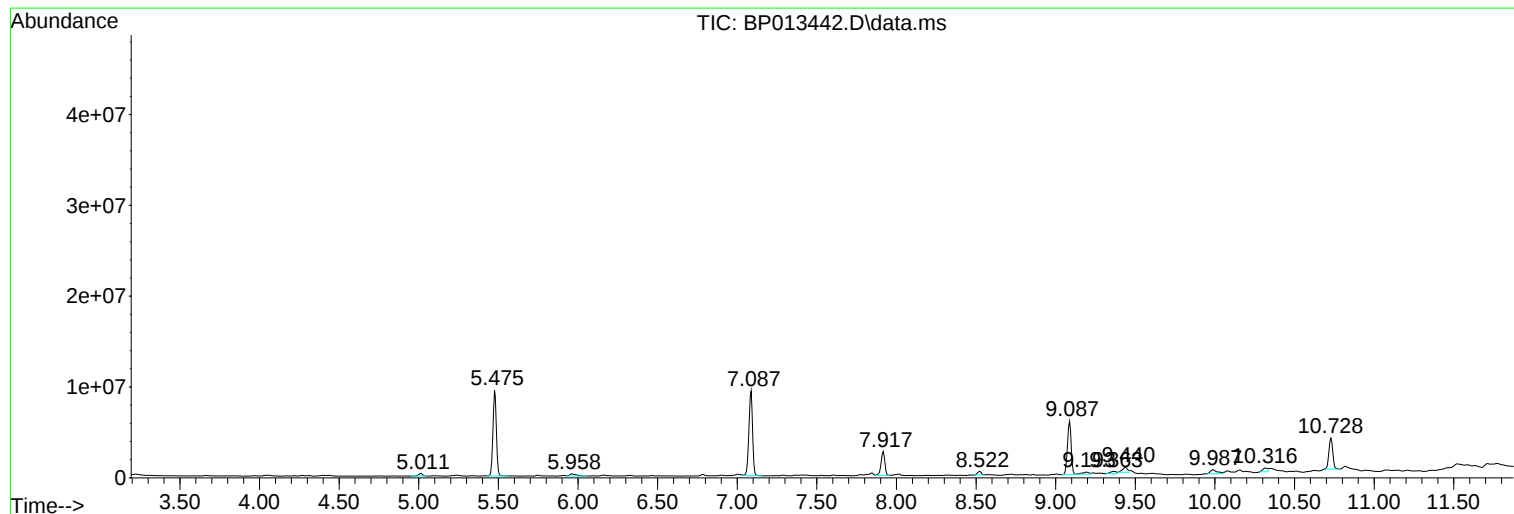

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013442.D
Acq On : 11 Jan 2023 14:12
Operator : CG/JU
Sample : 01051-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11933

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011123\
Data File : BP013442.D
Acq On : 11 Jan 2023 14:12
Operator : CG/JU
Sample : 01051-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11933

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------