
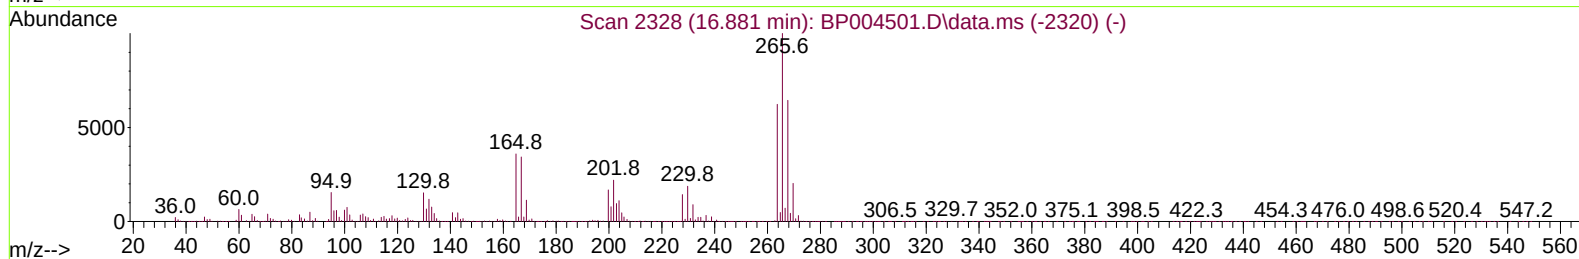
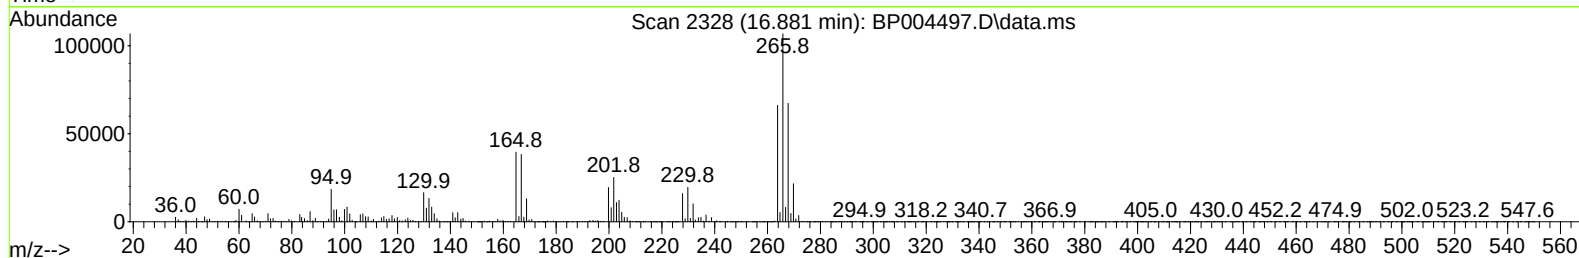


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
 Data File : BP004497.D
 Acq On : 12 Jan 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 03:56:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 12 15:19:32 2021
 Response via : Initial Calibration

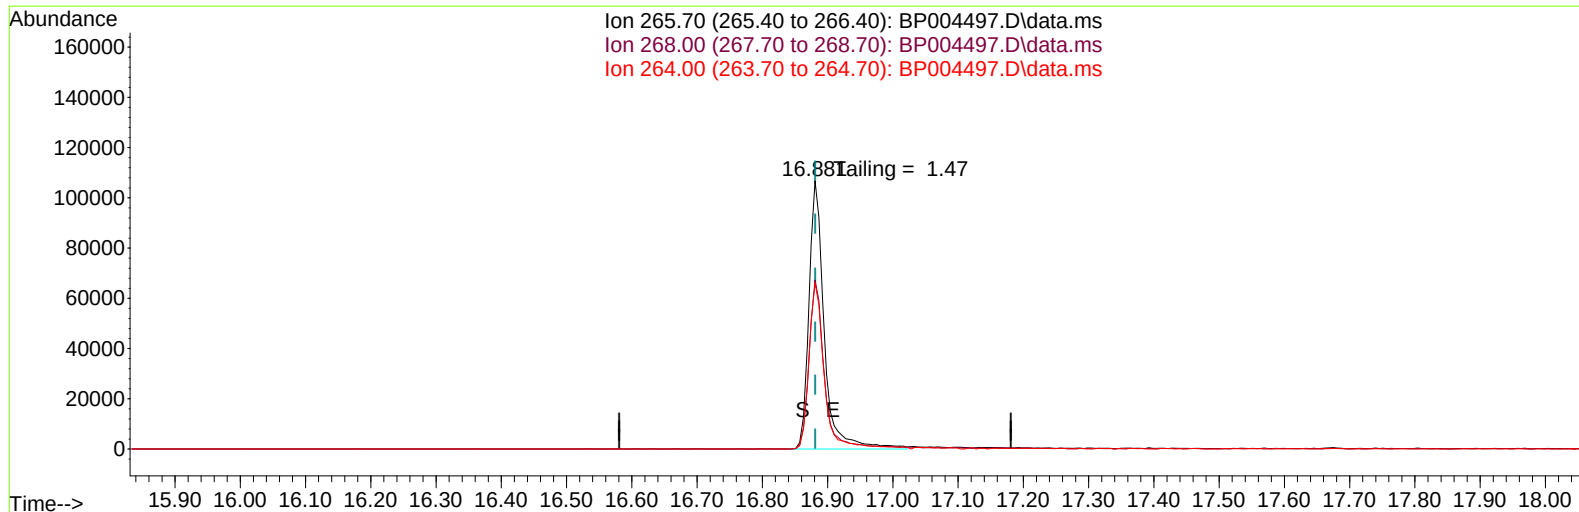

TIC: BP004497.D\data.ms

(70) Pentachlorophenol (C)




16.881min (-0.000) 121360.86 ng

response 176502

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.94
264.00	63.30	66.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
 Data File : BP004497.D
 Acq On : 12 Jan 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 03:56:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 12 15:19:32 2021
 Response via : Initial Calibration

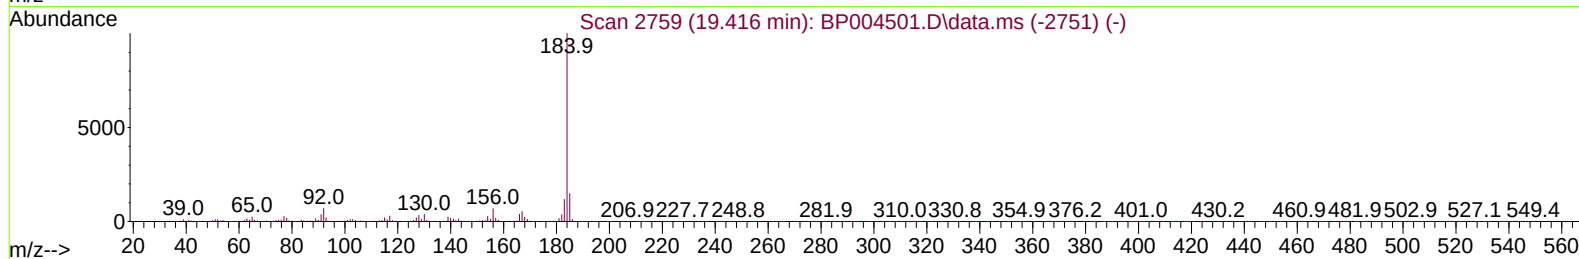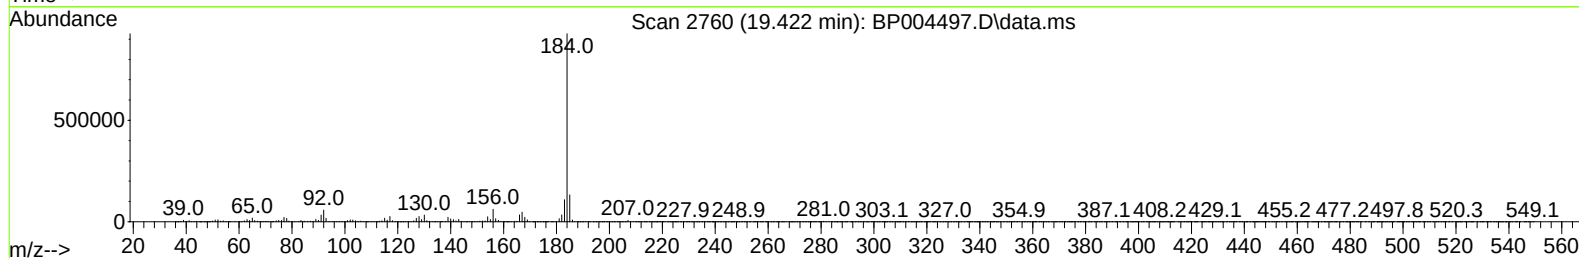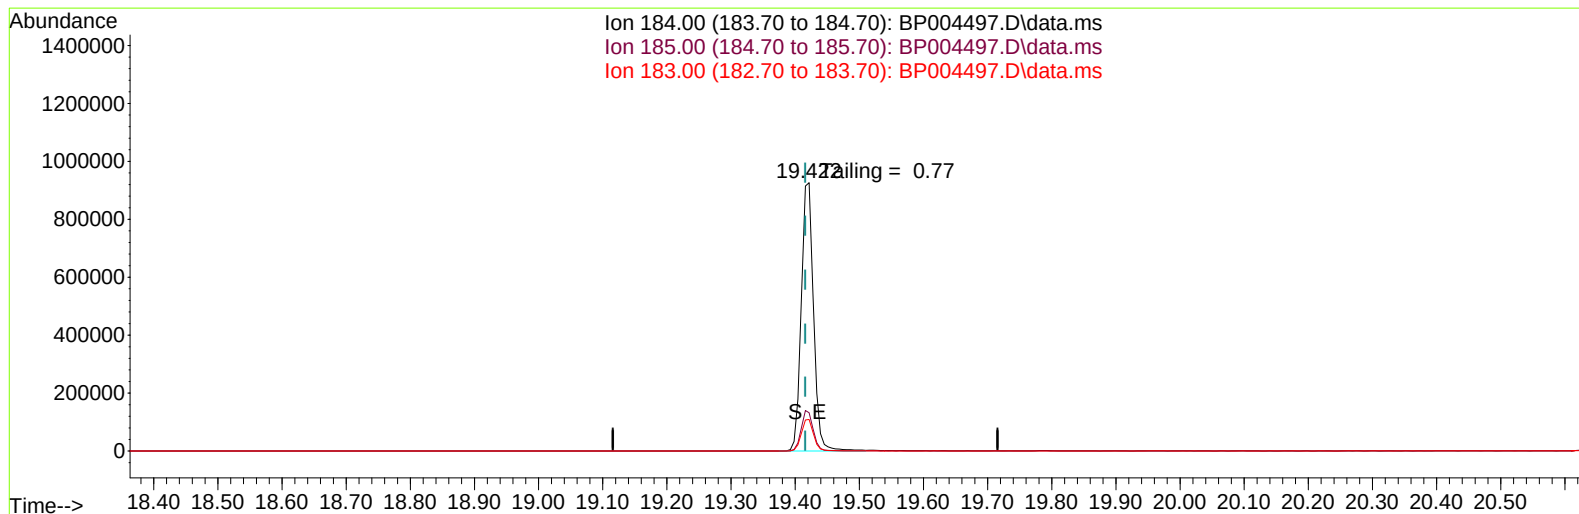

TIC: BP004497.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 67174.43 ng

response 1242536

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.27
183.00	12.00	11.77
0.00	0.00	0.00