
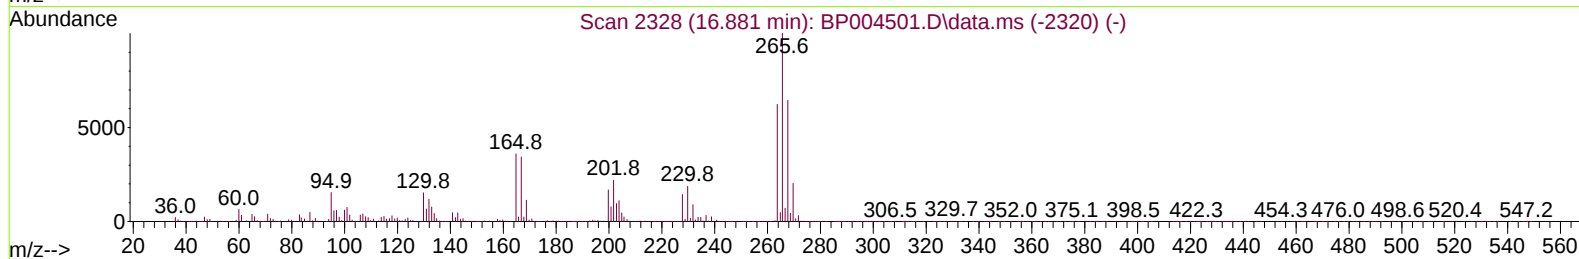
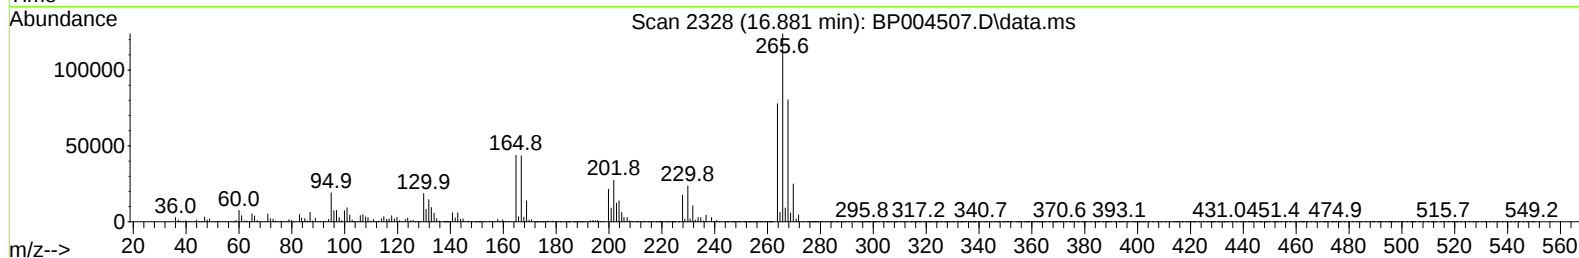


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004507.D
Acq On : 12 Jan 2021 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 04:59:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 12 15:19:32 2021
Response via : Initial Calibration

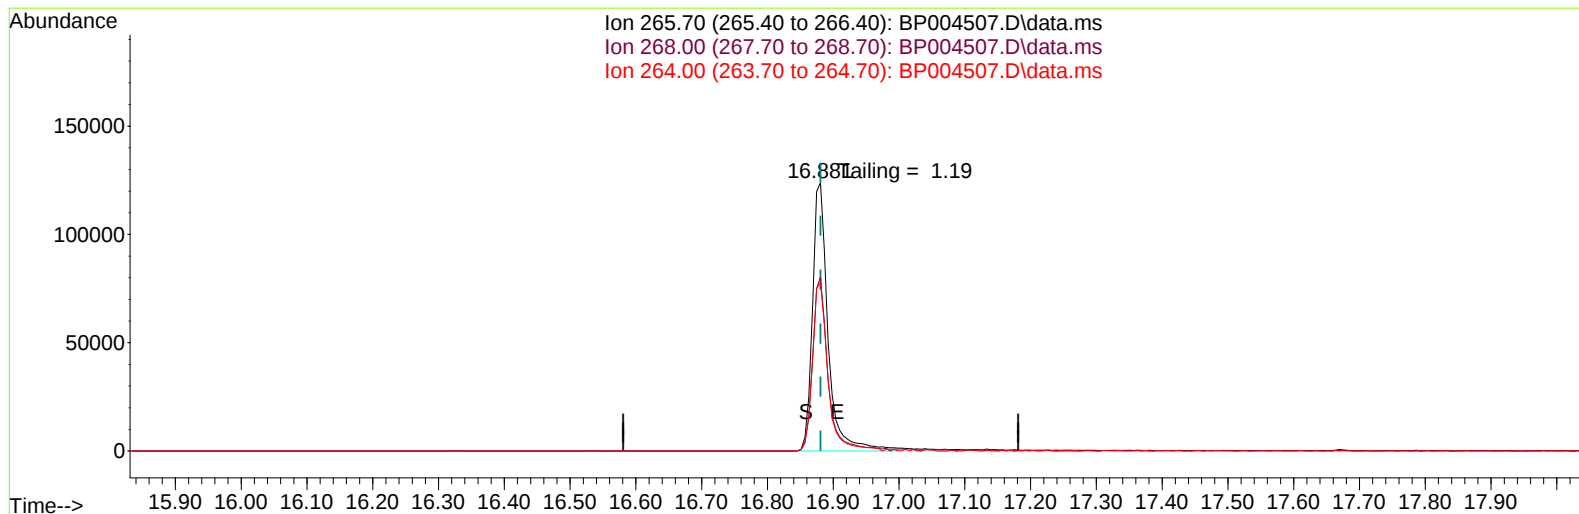

TIC: BP004507.D\data.ms

(70) Pentachlorophenol (C)




16.881min (-0.000) 761592.13 ng

response 207339

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	69.51
264.00	63.30	67.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004507.D
Acq On : 12 Jan 2021 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 04:59:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 12 15:19:32 2021
Response via : Initial Calibration

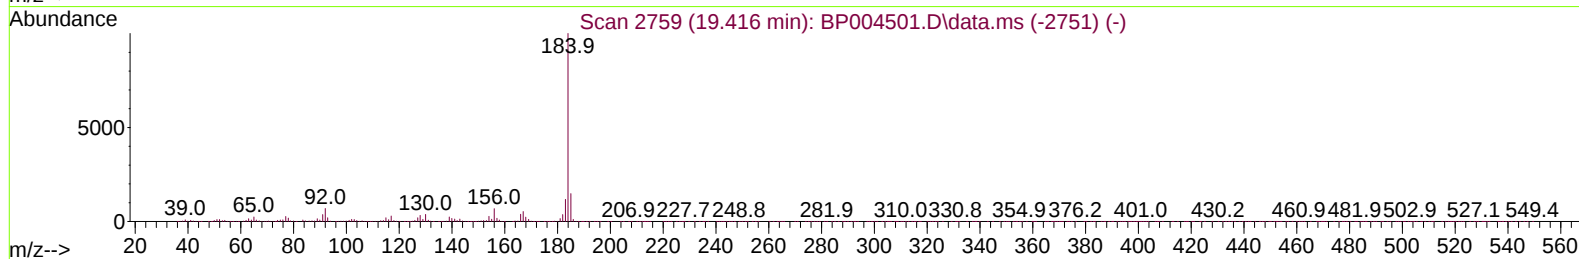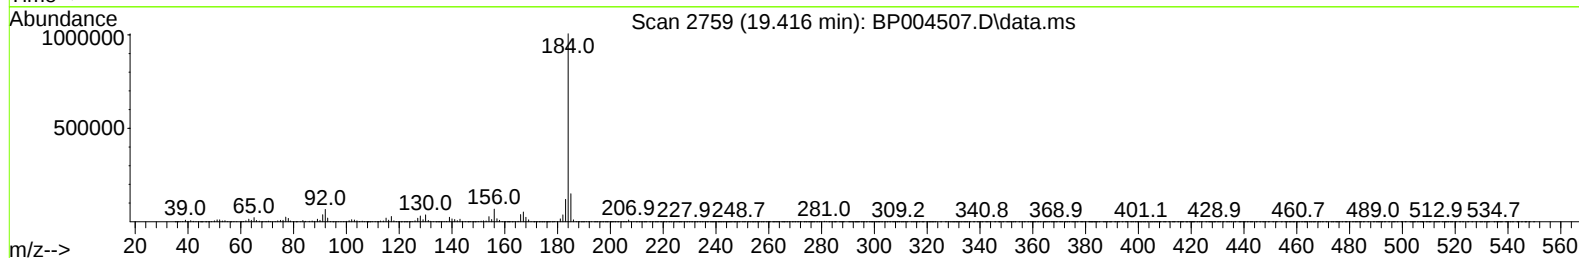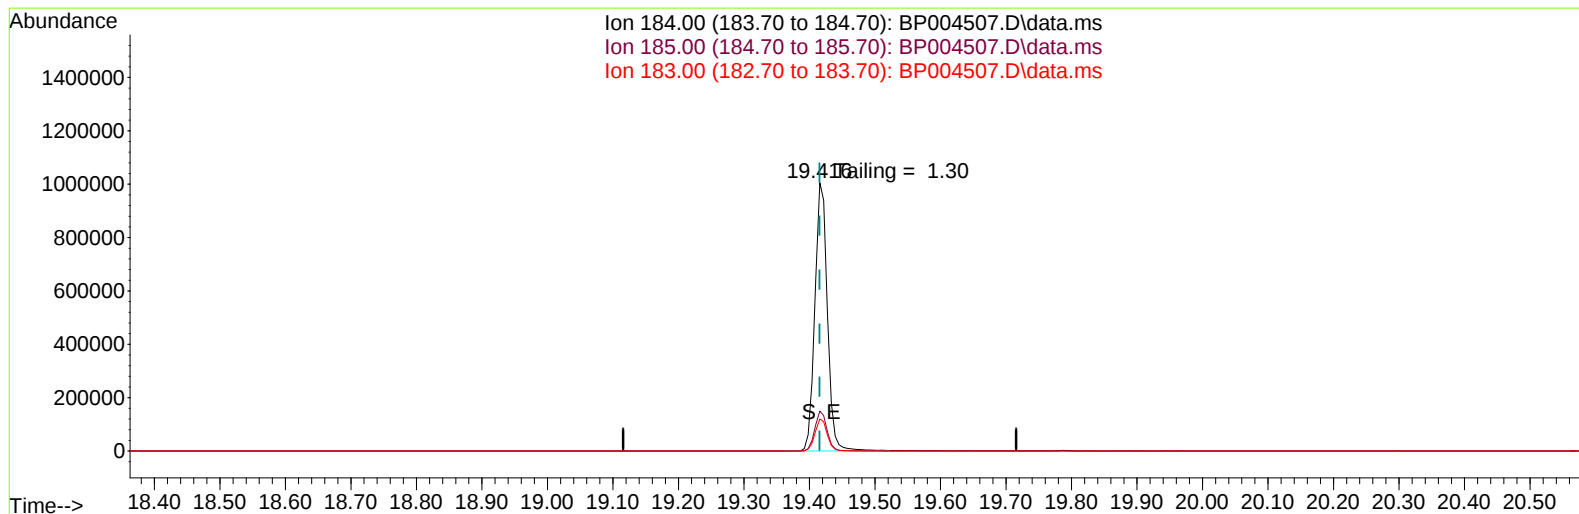

TIC: BP004507.D\data.ms

(77) Benzidine**19.416min (-0.000) 476650.92 ng****response 1334350**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.91
183.00	12.00	11.92
0.00	0.00	0.00