

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
 Data File : BP004506.D
 Acq On : 12 Jan 2021 15:53
 Operator : CG/JU
 Sample : PB134031BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB134031BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	370	377	396	rBV	2743102	4077336	31.73%	7.929%
2	6.987	638	646	665	rBV	2530317	4065866	31.64%	7.907%
3	7.816	779	787	801	rBV	583519	968646	7.54%	1.884%
4	8.975	975	984	999	rBV	1556364	2704147	21.04%	5.259%
5	10.610	1252	1262	1276	rBV	762760	1336088	10.40%	2.598%
6	13.081	1674	1682	1695	rBV	5013073	7270802	56.58%	14.140%
7	14.463	1910	1917	1932	rBV	1240397	1909786	14.86%	3.714%
8	15.963	2165	2172	2197	rBV4	4126206	6137651	47.76%	11.936%
9	17.228	2379	2387	2400	rBV	1701732	2464300	19.18%	4.792%
10	19.792	2817	2823	2836	rBV	10395815	12851413	100.00%	24.993%
11	20.992	3022	3027	3031	rBV	133685	232563	1.81%	0.452%
12	21.045	3032	3036	3040	rVV	197903	265982	2.07%	0.517%
13	21.092	3040	3044	3052	rVV	538706	712603	5.54%	1.386%
14	21.322	3077	3083	3089	rBV	2447386	3160721	24.59%	6.147%
15	23.674	3476	3483	3493	rVB2	1558993	3263032	25.39%	6.346%




Sum of corrected areas: 51420936

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004506.D
Acq On : 12 Jan 2021 15:53
Operator : CG/JU
Sample : PB134031BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB134031BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

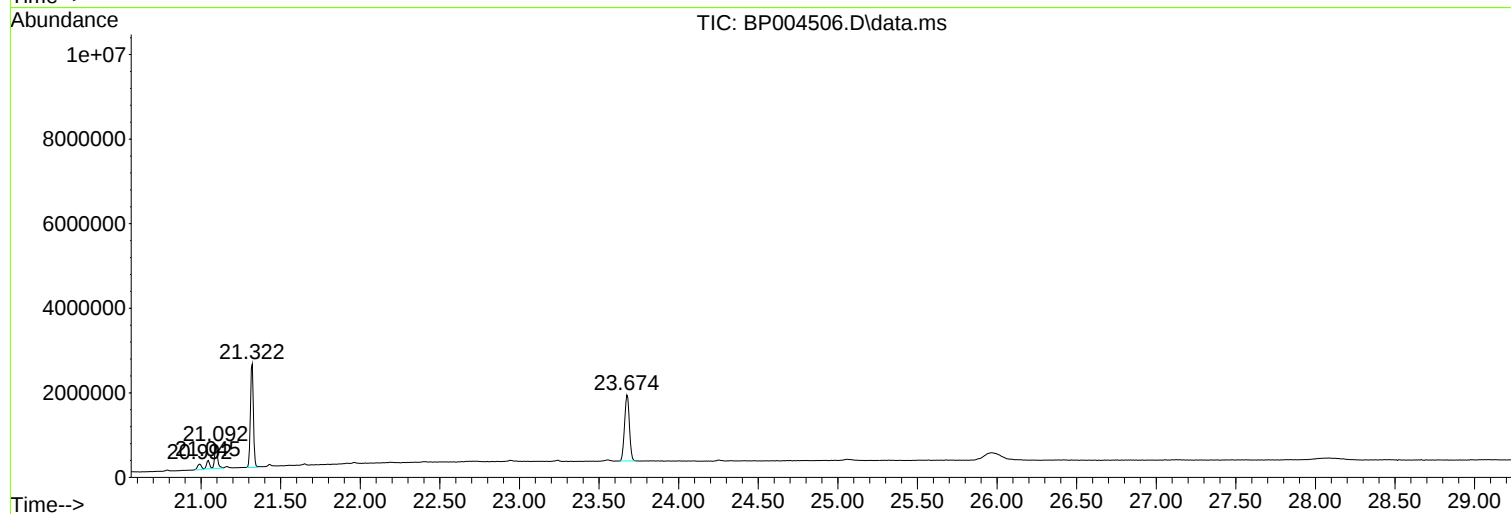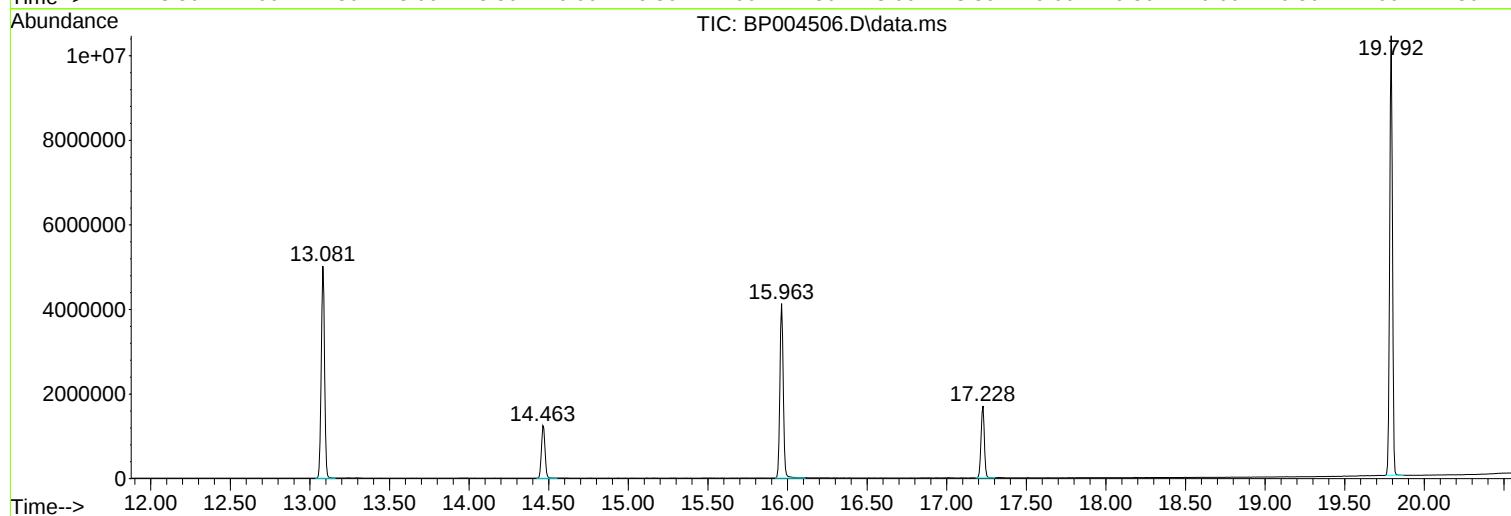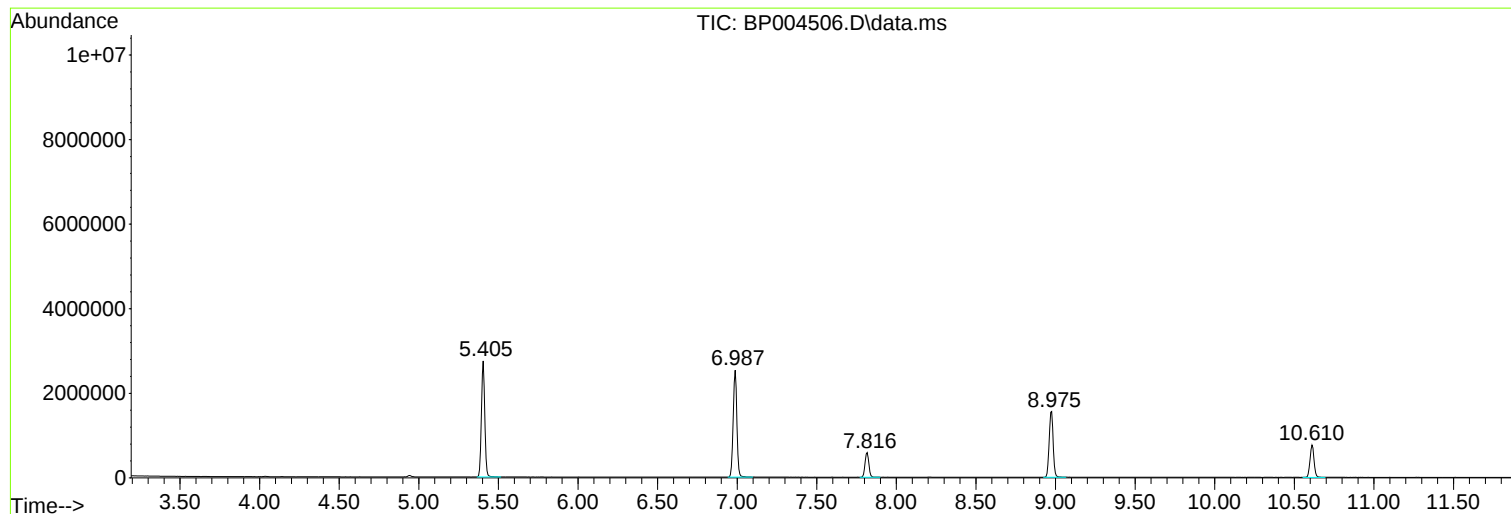

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004506.D
Acq On : 12 Jan 2021 15:53
Operator : CG/JU
Sample : PB134031BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB134031BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	4.51 ng	712603	Chrysene-d12	21.322

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	86
2			2,2'-(Ethane-1,2-diylbis(oxy))bi...	358	C20H22O6	1000366-99-4	78
3			2-(2-(2-Methoxyethoxy)ethoxy)eth...	268	C14H20O5	1000366-99-1	74
4			3-Benzoylamino-2-benzyl-butyric ...	311	C19H21NO3	1000193-12-7	64
5			1,3-Dioxolane, 2-(methoxymethyl)...	194	C11H14O3	1000156-71-2	64

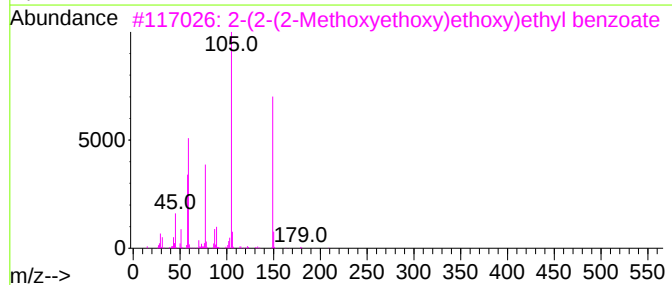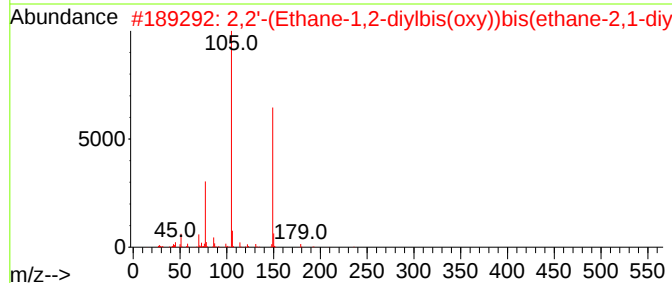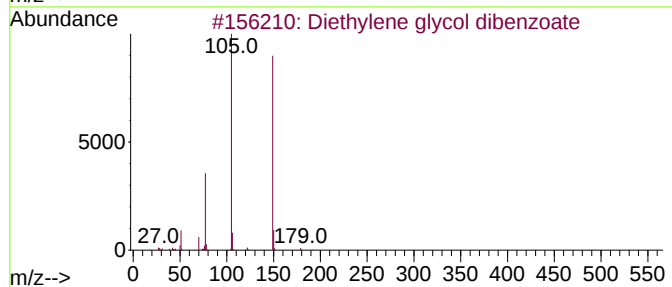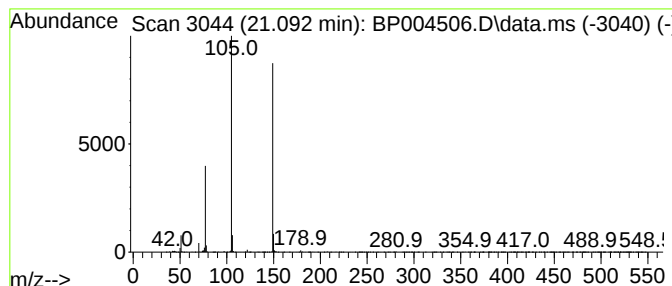

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004506.D
Acq On : 12 Jan 2021 15:53
Operator : CG/JU
Sample : PB134031BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB134031BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	21.092	4.5	ng	712603	5	21.322	3160720	20.0