

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
 Data File : BP004523.D
 Acq On : 13 Jan 2021 01:35
 Operator : CG/JU
 Sample : M1059-01 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TR-04-010821

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	370	377	386	rBV	467324	732111	18.23%	3.008%
2	6.987	633	646	662	rBV	450965	800231	19.92%	3.287%
3	7.816	778	787	797	rBV	820830	1356526	33.77%	5.573%
4	8.969	977	983	992	rBV	284357	484164	12.05%	1.989%
5	10.610	1251	1262	1273	rBV	1112069	1939422	48.28%	7.967%
6	13.081	1673	1682	1691	rBV	894583	1370307	34.11%	5.629%
7	13.916	1820	1824	1834	rVB	27765	46577	1.16%	0.191%
8	14.463	1909	1917	1930	rBV	1825251	2781018	69.23%	11.424%
9	15.963	2166	2172	2180	rBV	722680	1067447	26.57%	4.385%
10	17.227	2380	2387	2393	rBV	2273739	3305631	82.29%	13.580%
11	18.998	2685	2688	2691	rBV4	93307	110432	2.75%	0.454%
12	19.786	2817	2822	2828	rBV	1728837	2158861	53.75%	8.869%
13	21.092	3041	3044	3050	rBV	424994	540916	13.47%	2.222%
14	21.315	3078	3082	3088	rVB	2802822	3632162	90.42%	14.921%
15	23.674	3477	3483	3493	rVB2	2004537	4016831	100.00%	16.501%




Sum of corrected areas: 24342636

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004523.D
Acq On : 13 Jan 2021 01:35
Operator : CG/JU
Sample : M1059-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR-04-010821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

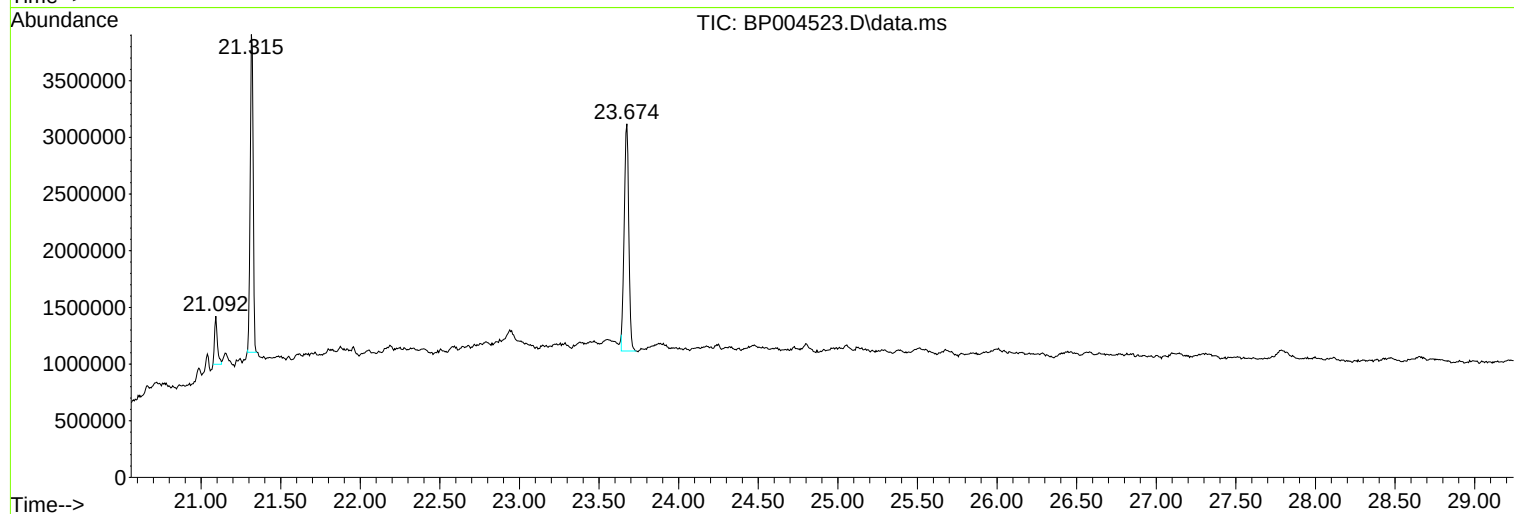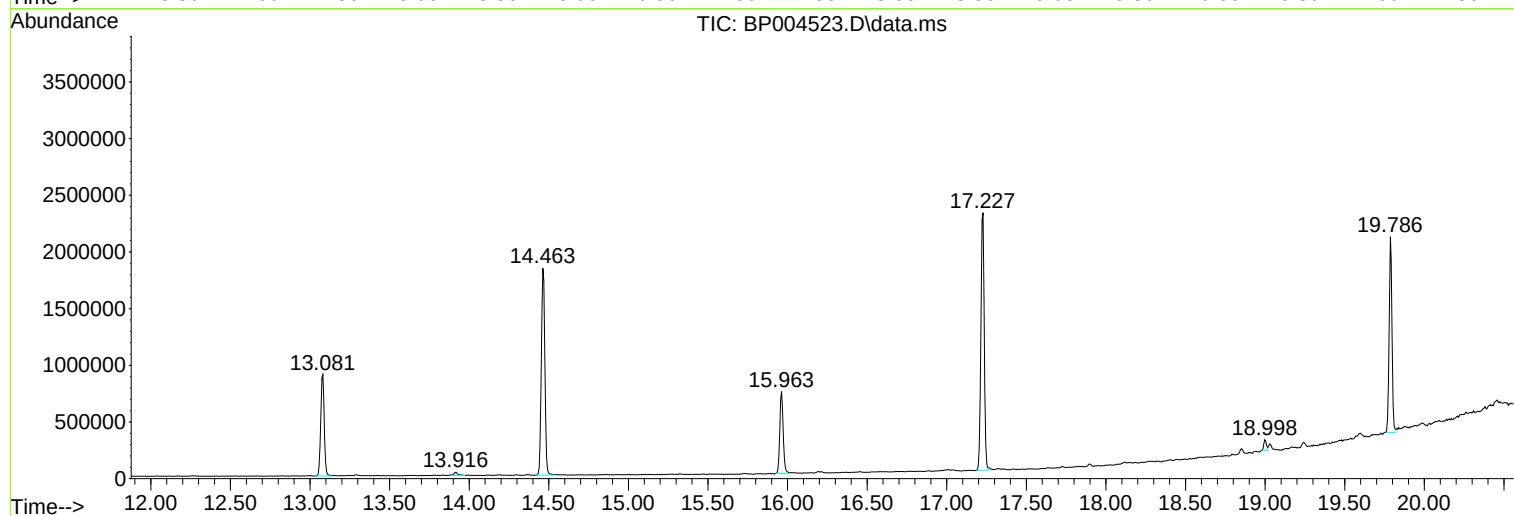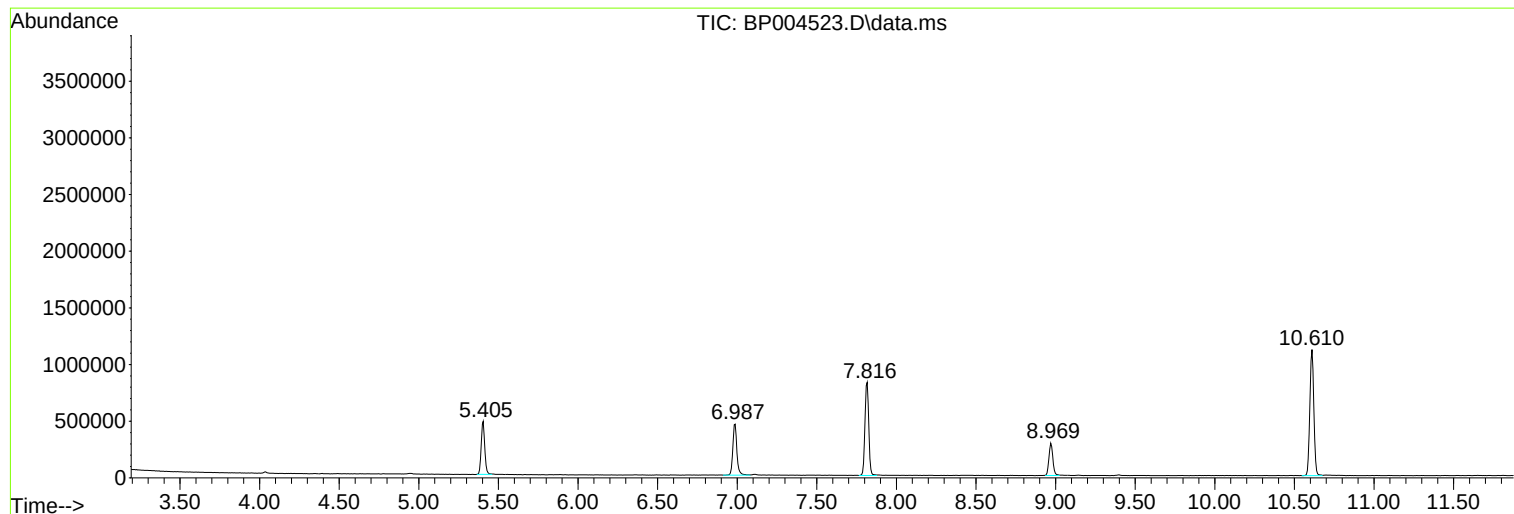

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004523.D
Acq On : 13 Jan 2021 01:35
Operator : CG/JU
Sample : M1059-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR-04-010821










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,5,8,11-Tetraoxatridecan-1... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	2.98 ng	540916	Chrysene-d12	21.316

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,5,8,11-Tetraoxatridecan-13-yl ...	312	C16H24O6	1000366-96-7	78		
2	2,2'-(Ethane-1,2-diylbis(oxy))bi...	358	C20H22O6	1000366-99-4	78		
3	Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	64		
4	Benzoic acid, 2-(4-nitrophenoxy)...	287	C15H13NO5	1000368-92-7	64		
5	1,3-Dioxolane, 2-(methoxymethyl)...	194	C11H14O3	1000156-71-2	64		

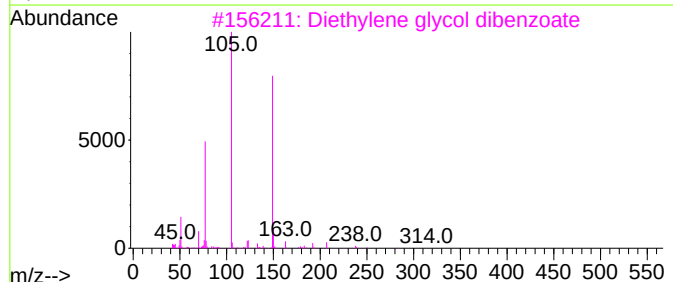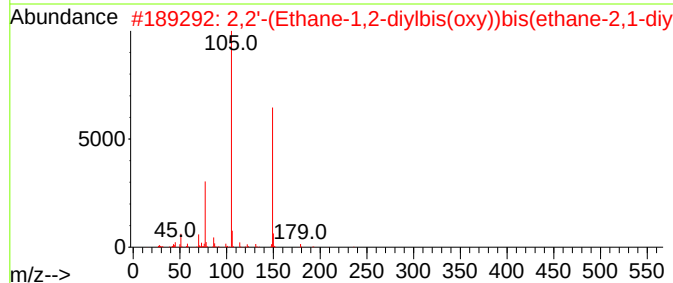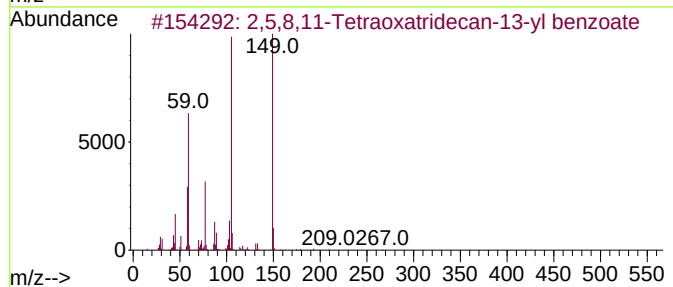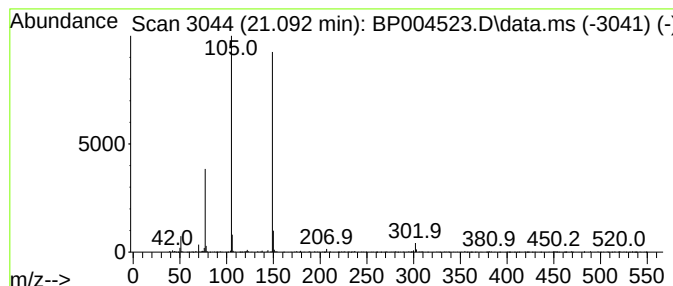

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
Data File : BP004523.D
Acq On : 13 Jan 2021 01:35
Operator : CG/JU
Sample : M1059-01 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR-04-010821

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,5,8,11-Tetrao...	21.092	3.0	ng	540916	5	21.316	3632160	20.0