
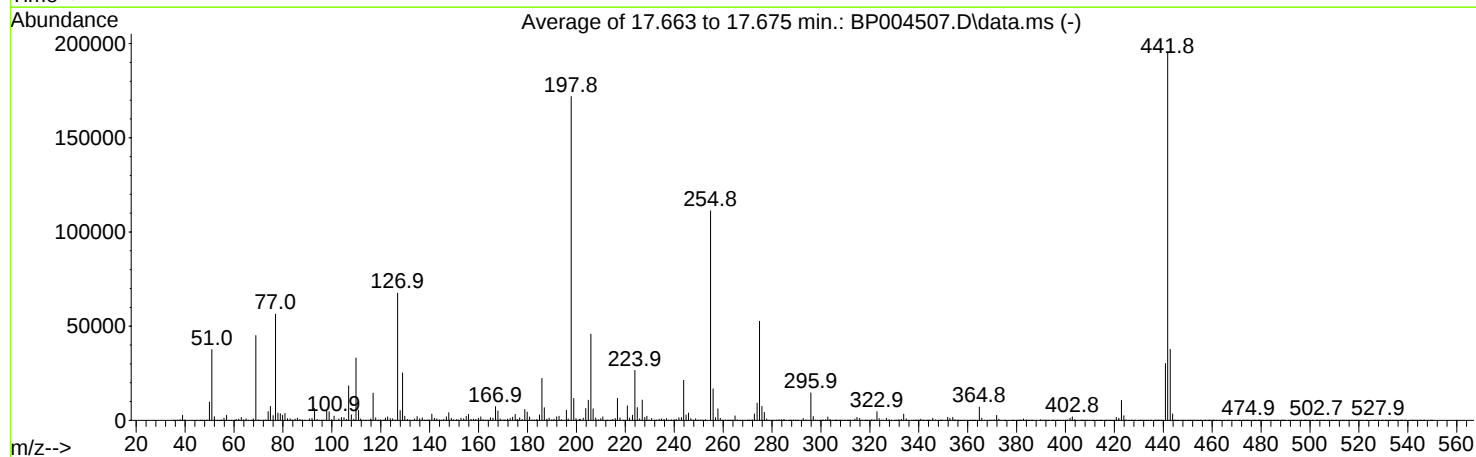


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011221\
 Data File : BP004507.D
 Acq On : 12 Jan 2021 16:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 12 15:19:32 2021

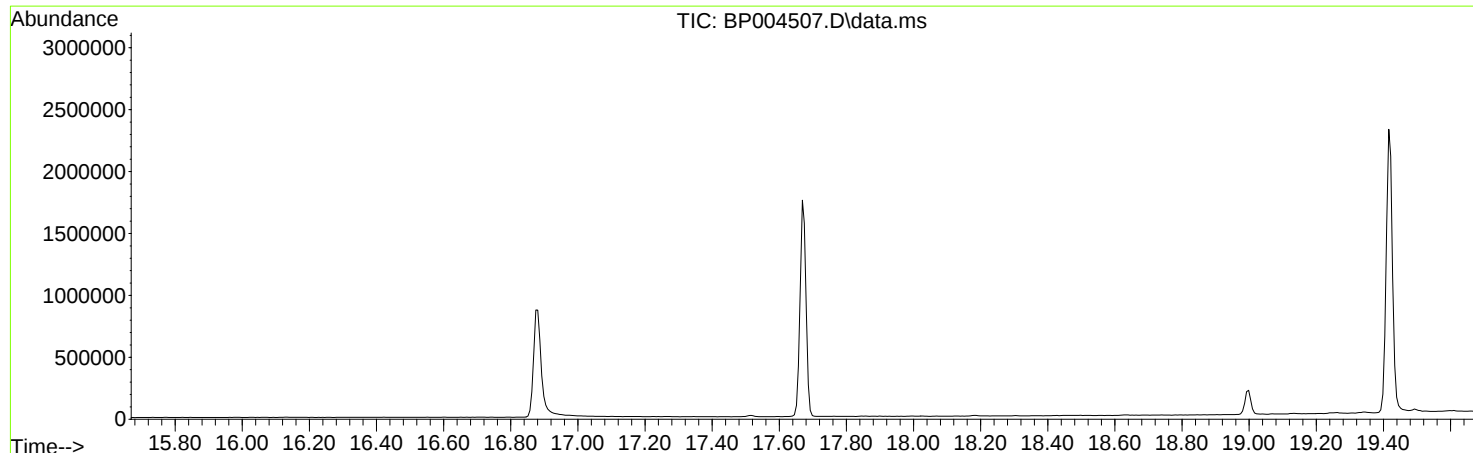

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.9	37621	PASS
68	69	0.00	2	2.0	892	PASS
69	198	0.00	100	26.2	45034	PASS
70	69	0.00	2	0.6	271	PASS
127	198	10	80	39.3	67556	PASS
197	198	0.00	2	0.1	165	PASS
198	198	100	100	100.0	171925	PASS
199	198	5	9	6.8	11607	PASS
275	198	10	60	30.6	52605	PASS
365	198	1	100	4.1	7059	PASS
441	198	0.01	100	17.6	30208	PASS
442	442	100	100	100.0	195281	PASS
443	442	15	24	19.3	37739	PASS