
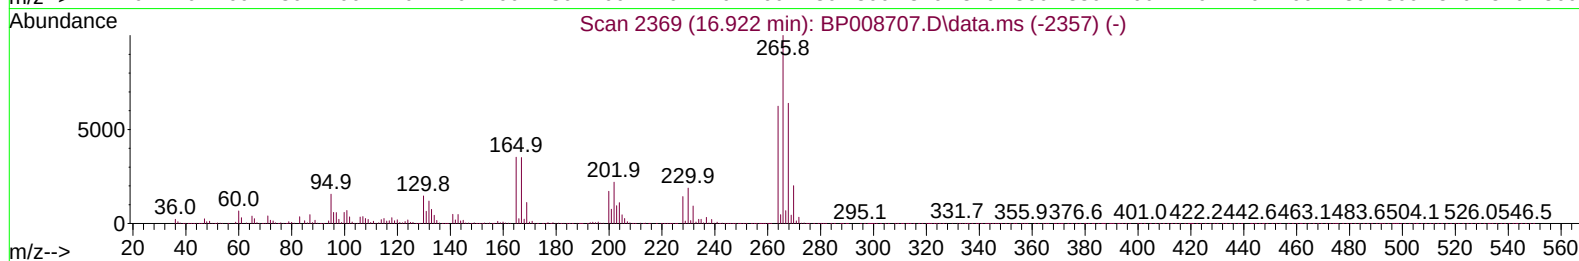
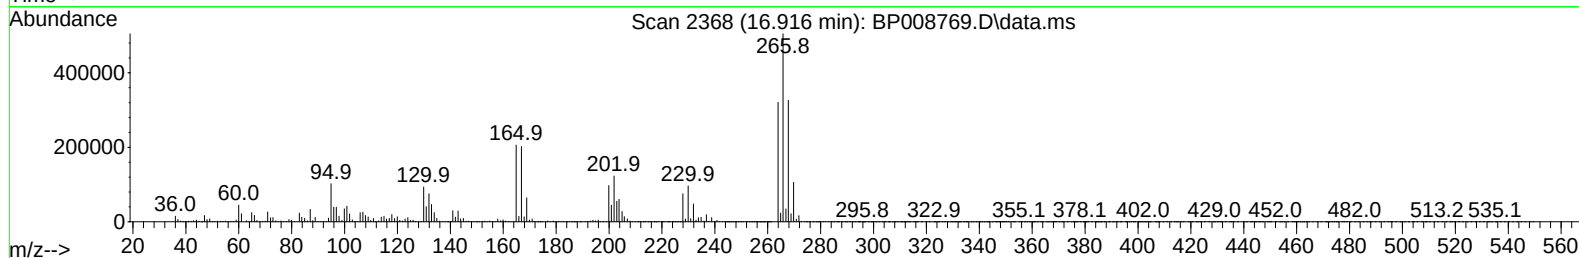


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
 Data File : BP008769.D
 Acq On : 12 Jan 2022 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 16:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 12 00:18:56 2022
 Response via : Initial Calibration

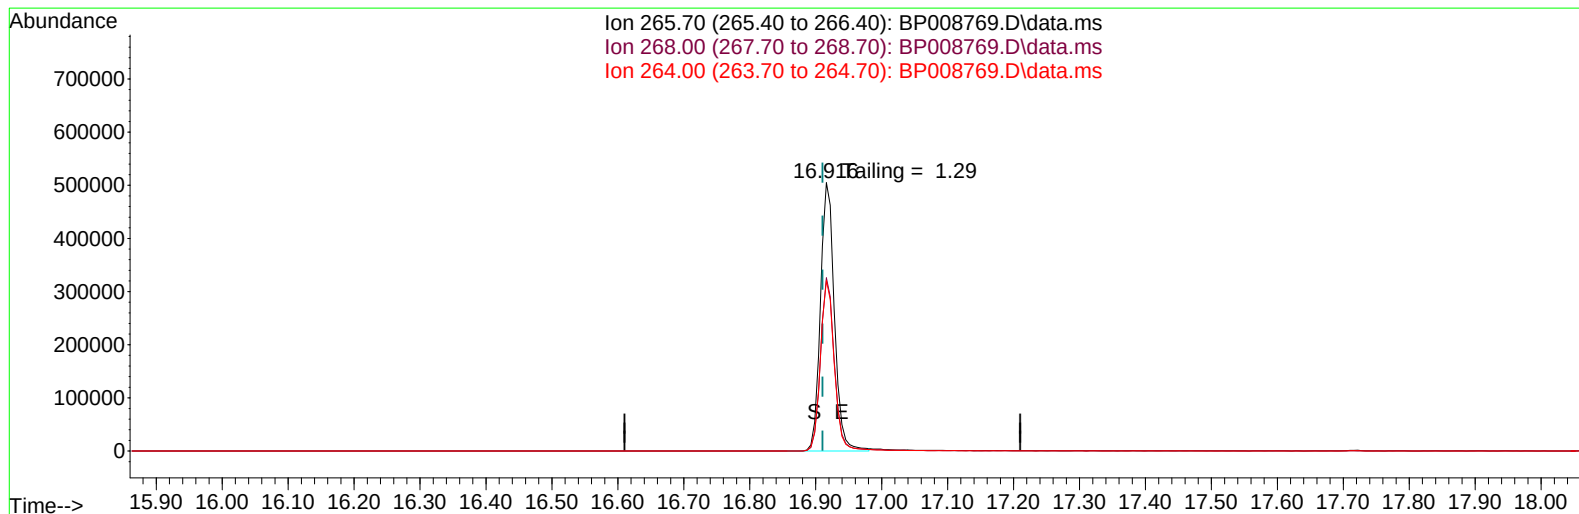

TIC: BP008769.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.006) 690978.20 ng

response 754139

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.57
264.00	62.90	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
 Data File : BP008769.D
 Acq On : 12 Jan 2022 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 16:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 12 00:18:56 2022
 Response via : Initial Calibration

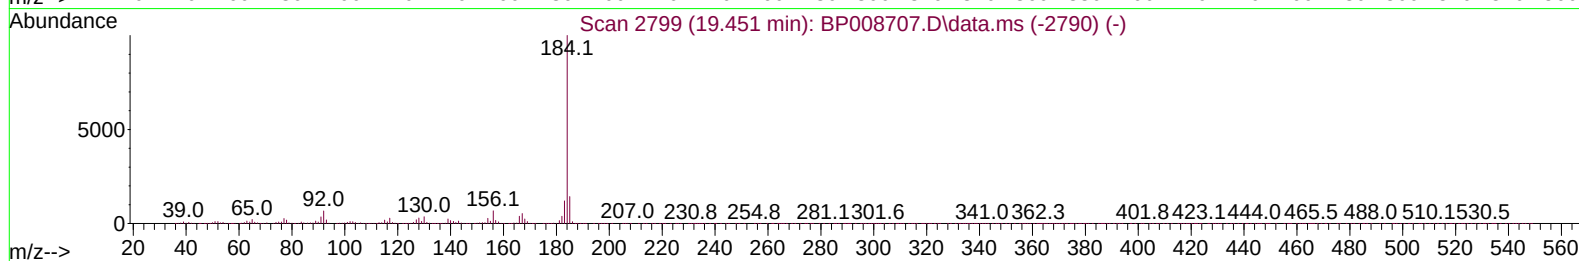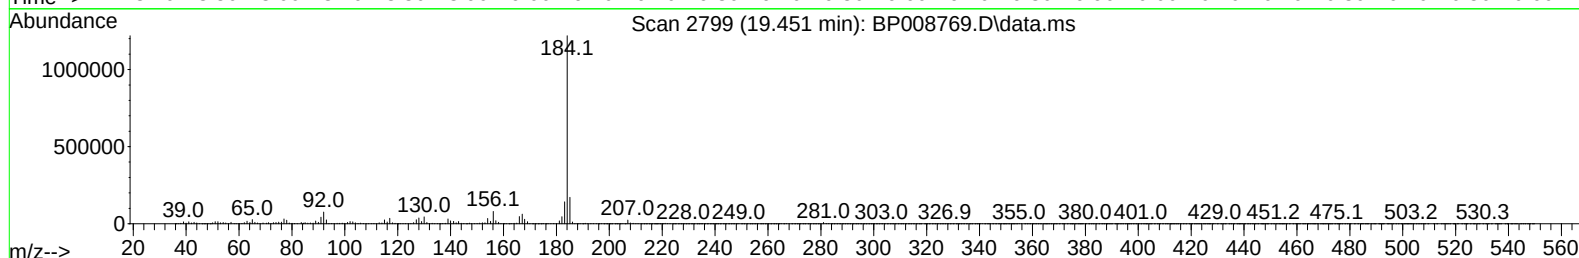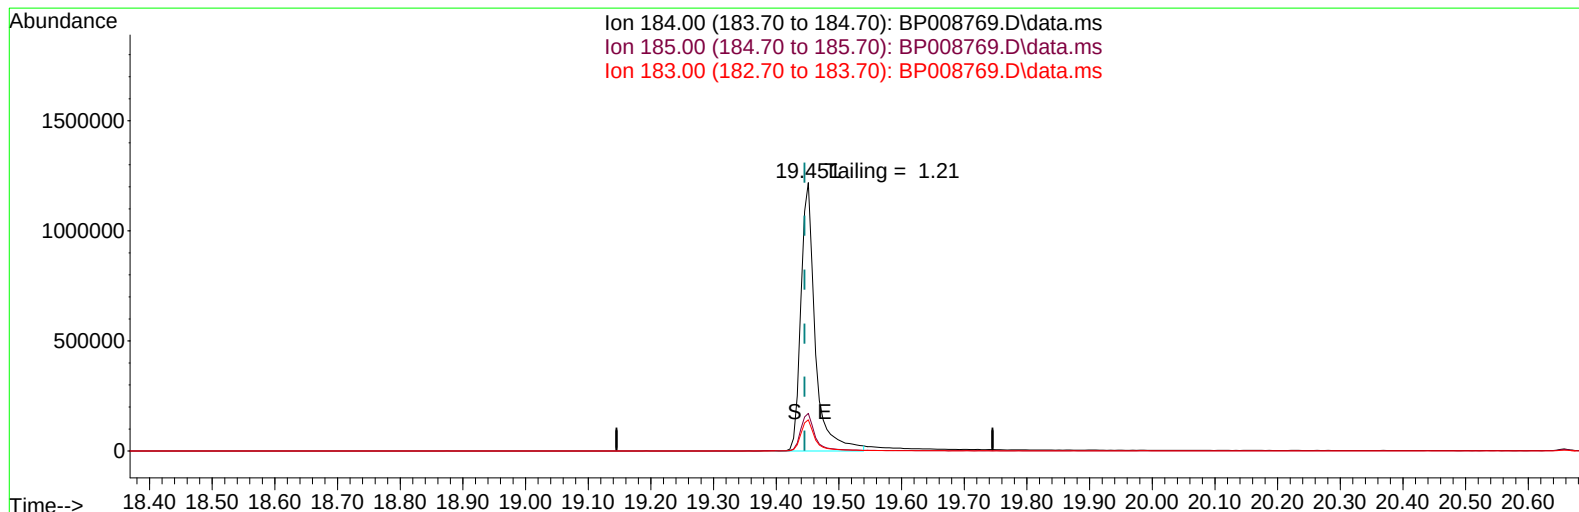

TIC: BP008769.D\data.ms

(77) Benzidine**19.451min (+ 0.006) 303856.09 ng****response 2028250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.02
183.00	11.90	11.65
0.00	0.00	0.00