

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
 Data File : BP008771.D
 Acq On : 12 Jan 2022 13:23
 Operator : CG/JU
 Sample : PB141938BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141938BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	25	rVB	226502	306329	1.29%	0.328%
2	5.452	412	419	435	rBV	5390571	8178934	34.51%	8.755%
3	7.046	682	690	709	rBV	5000305	8162157	34.44%	8.737%
4	7.869	822	830	839	rBV	1123879	1838218	7.76%	1.968%
5	9.028	1018	1027	1041	rBV	3036783	5267247	22.22%	5.638%
6	10.669	1299	1306	1316	rBV	1434242	2484289	10.48%	2.659%
7	13.128	1715	1724	1738	rBV	8841911	13446381	56.73%	14.394%
8	14.340	1919	1930	1943	rBV2	69309	242050	1.02%	0.259%
9	14.504	1951	1958	1970	rVB	2310358	3458199	14.59%	3.702%
10	15.998	2204	2212	2233	rBV	7275473	10577828	44.63%	11.323%
11	17.257	2419	2426	2439	rBV	2991819	4364698	18.42%	4.672%
12	19.822	2856	2862	2867	rBV	18933486	23701579	100.00%	25.371%
13	21.345	3116	3121	3132	rBV	3998856	5364925	22.64%	5.743%
14	21.463	3138	3141	3147	rBV	303940	396321	1.67%	0.424%
15	23.774	3527	3534	3545	rVB2	2711800	5630379	23.76%	6.027%


Sum of corrected areas: 93419534

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
Data File : BP008771.D
Acq On : 12 Jan 2022 13:23
Operator : CG/JU
Sample : PB141938BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141938BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

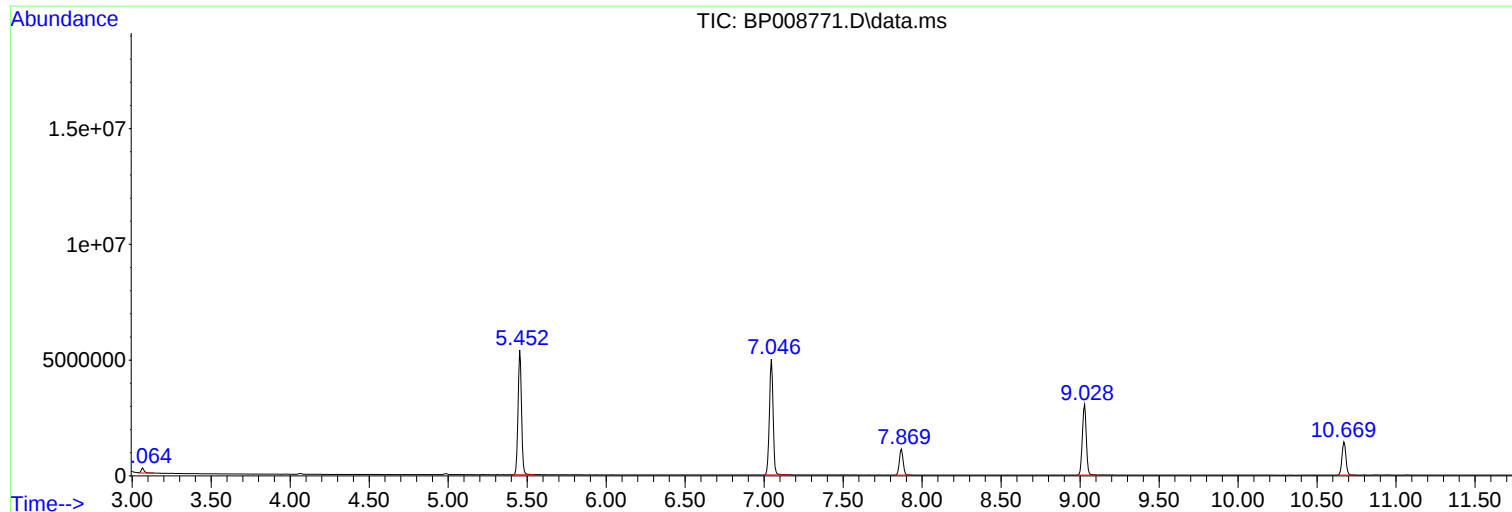

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
Data File : BP008771.D
Acq On : 12 Jan 2022 13:23
Operator : CG/JU
Sample : PB141938BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141938BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.064	3.33 ng	306329	1,4-Dichlorobenzene-d4	7.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

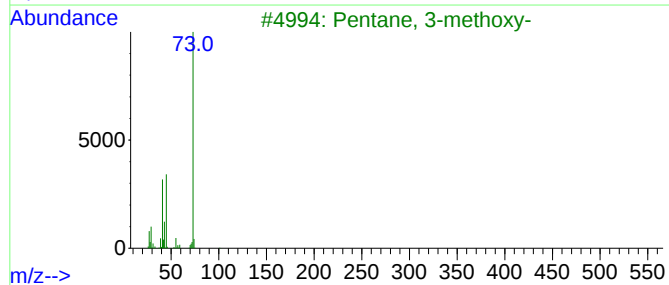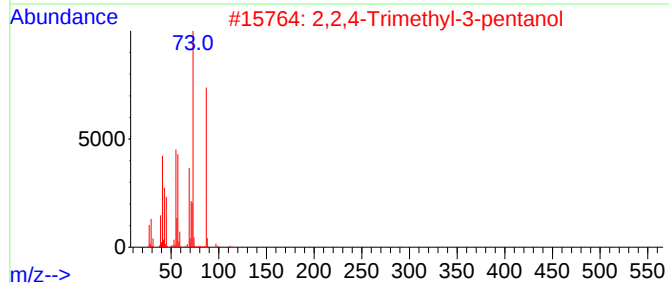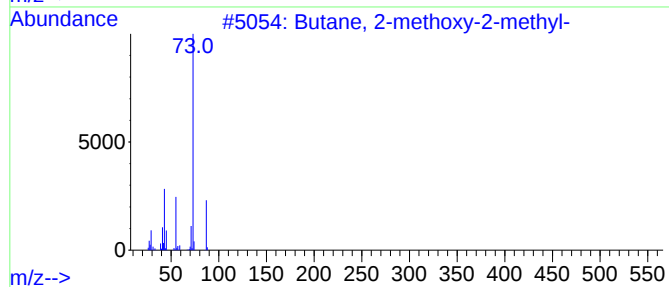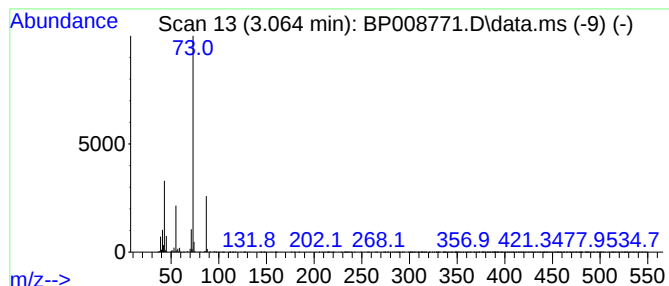

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
Data File : BP008771.D
Acq On : 12 Jan 2022 13:23
Operator : CG/JU
Sample : PB141938BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141938BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.064	3.3	ng	306329	1	7.869	1838220	20.0