
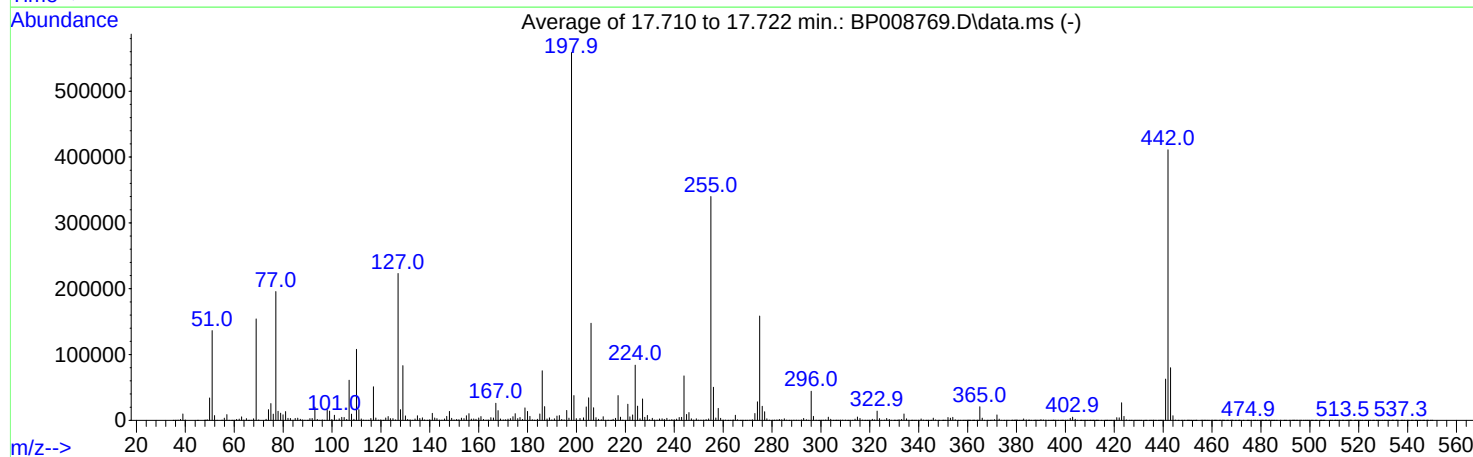


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
 Data File : BP008769.D
 Acq On : 12 Jan 2022 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 12 00:18:56 2022

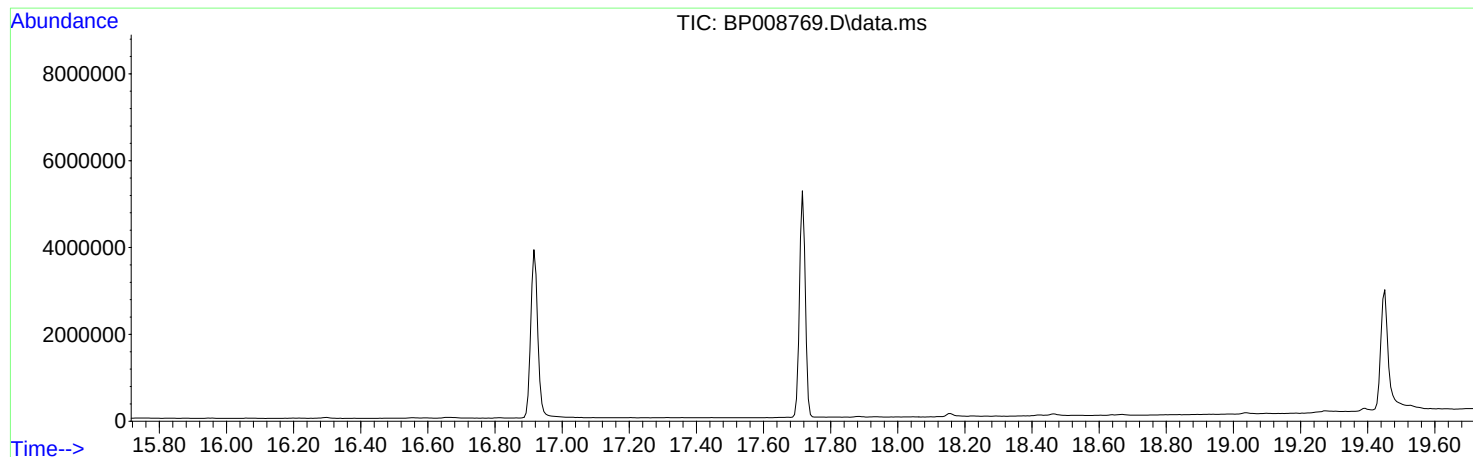


AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	136415	PASS
68	69	0.00	2	1.6	2460	PASS
69	198	0.00	100	27.6	154150	PASS
70	69	0.00	2	0.5	727	PASS
127	198	10	80	40.0	223267	PASS
197	198	0.00	2	0.6	3348	PASS
198	198	100	100	100.0	558857	PASS
199	198	5	9	6.7	37613	PASS
275	198	10	60	28.3	158421	PASS
365	198	1	100	3.7	20692	PASS
441	198	0.01	100	11.2	62784	PASS
442	442	100	100	100.0	411008	PASS
443	442	15	24	19.5	80072	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
Data File : BP008769.D
Acq On : 12 Jan 2022 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 12 16:17:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 12 00:18:56 2022
Response via : Initial Calibration

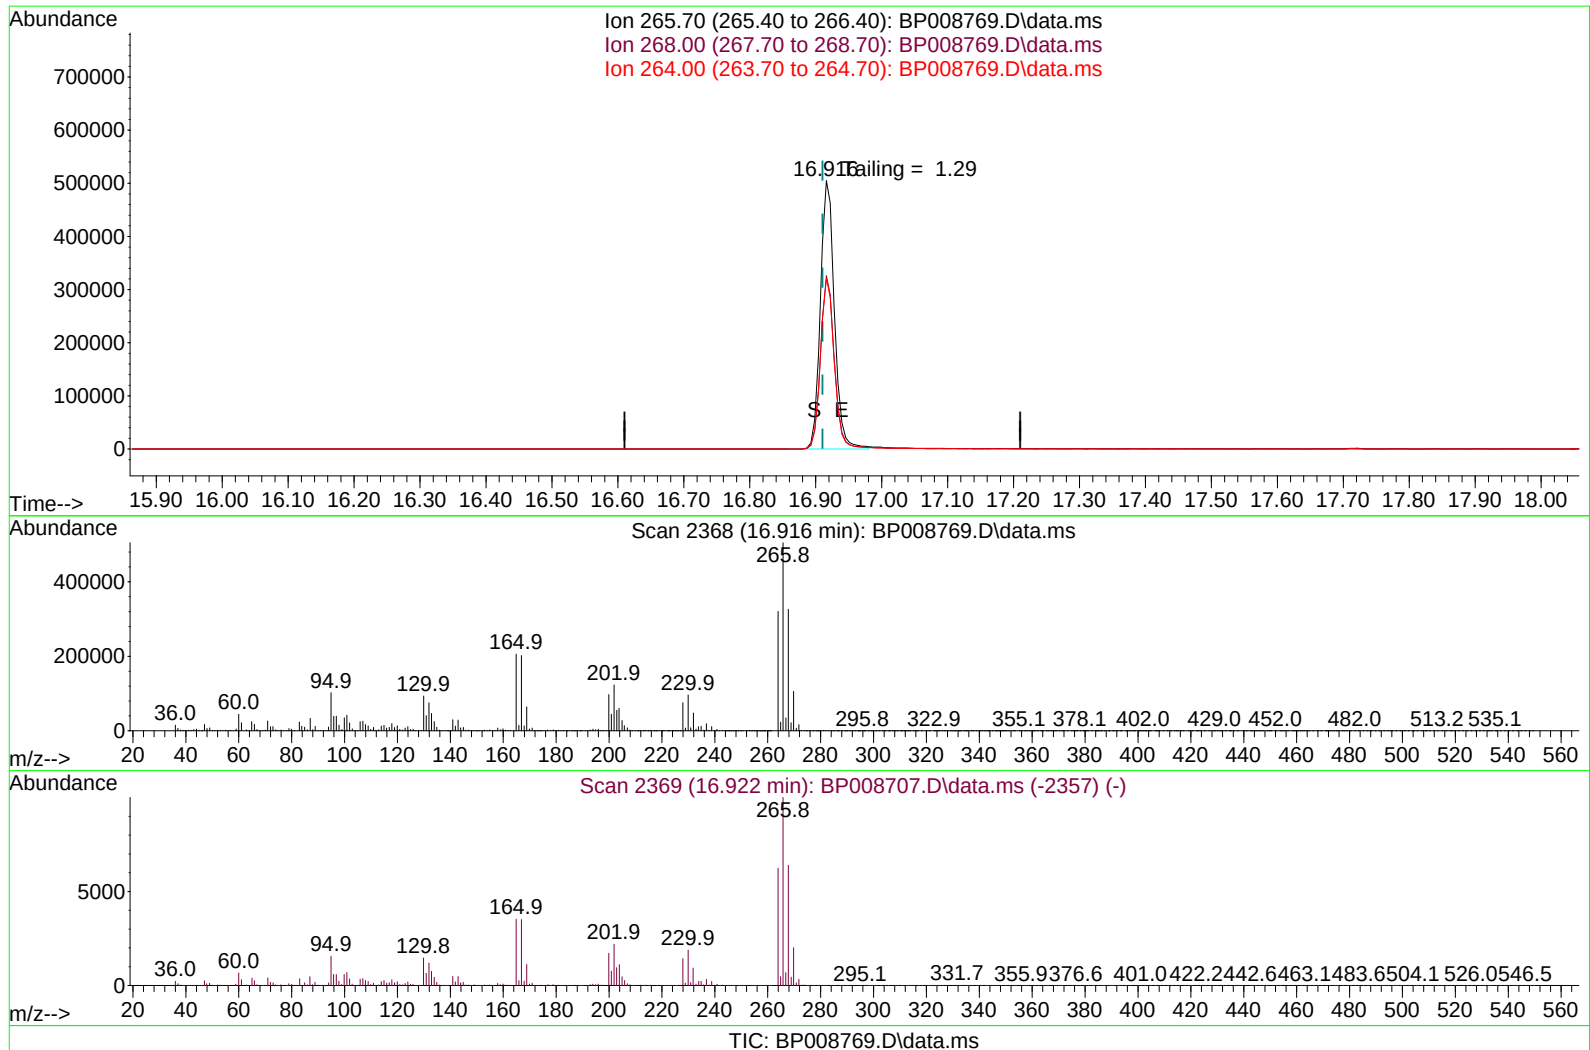

TIC: BP008769.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 690978.20 ng




response 754139

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.57
264.00	62.90	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011222\
Data File : BP008769.D
Acq On : 12 Jan 2022 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 12 16:17:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 12 00:18:56 2022
Response via : Initial Calibration

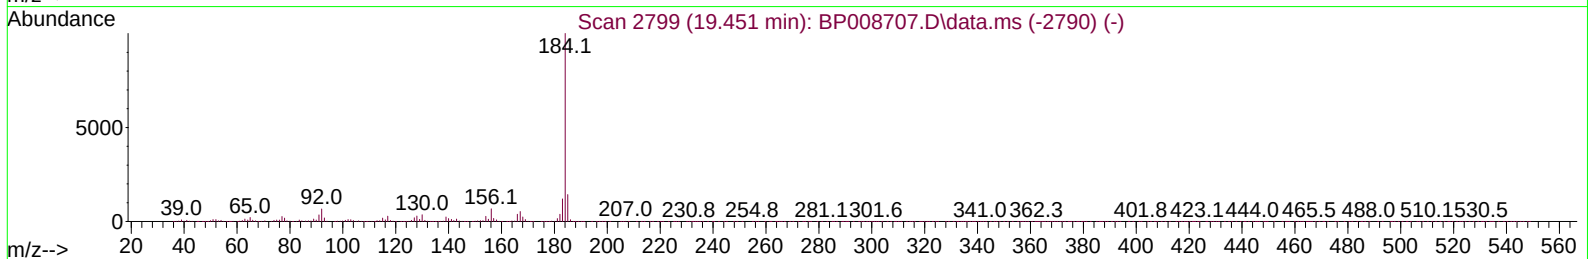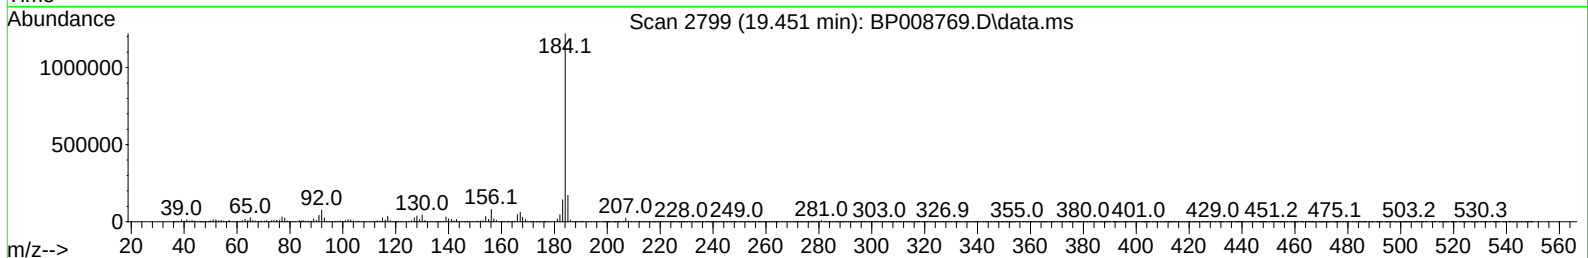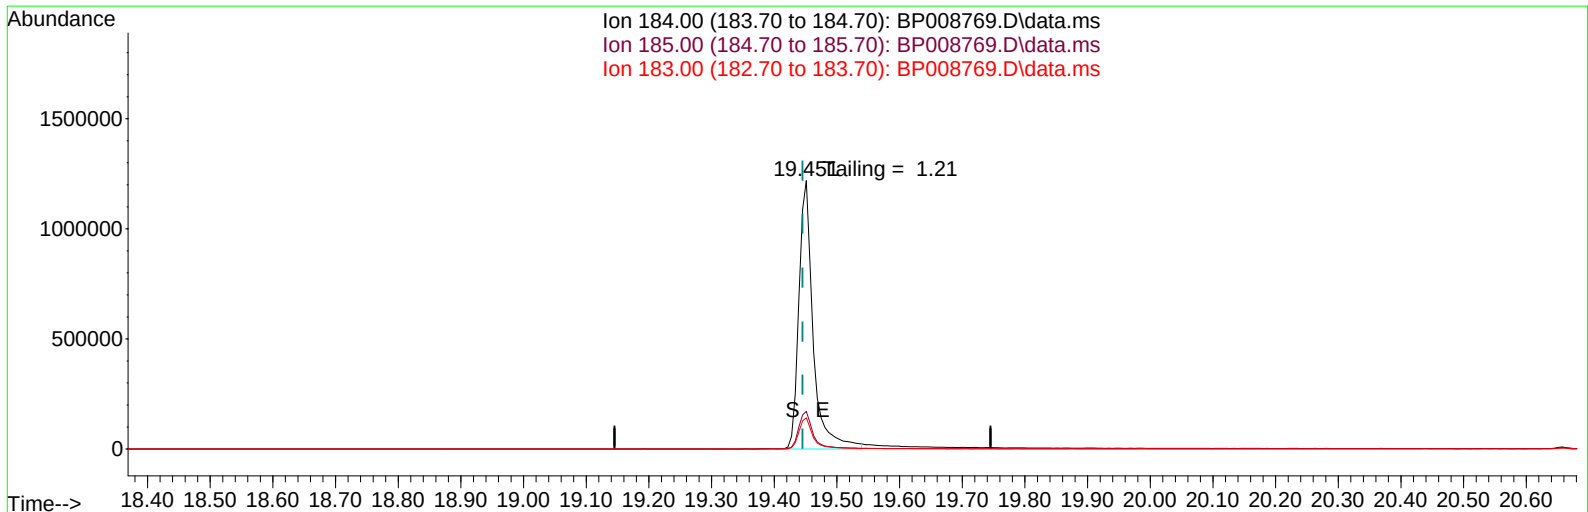

TIC: BP008769.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 303856.09 ng

response 2028250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.02
183.00	11.90	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2022	BNA_P	<u>BP008769.D</u>
Compound Name	Response	Retention Time
DDT	2011496	20.65
DDD	44593	20.22
DDE	3734	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48327	2059823	2.35

Instrument :
BNA_P
ClientSampleId :
DFTPP