
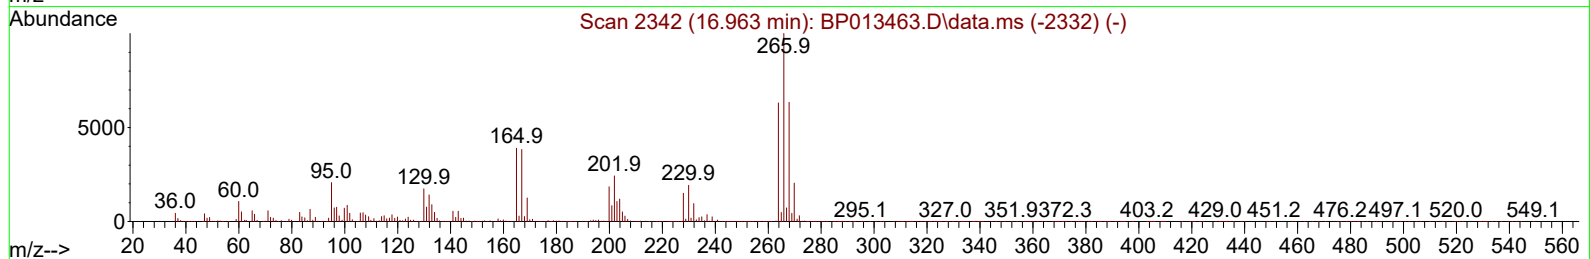
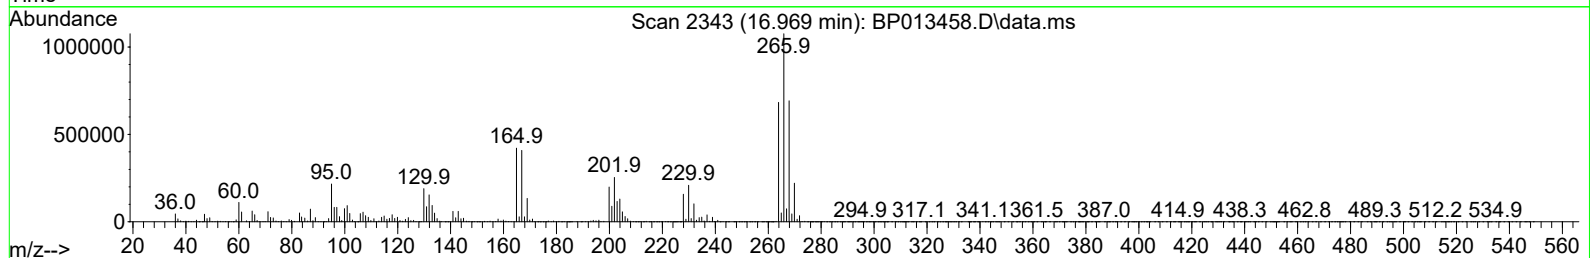


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011223\
Data File : BP013458.D
Acq On : 12 Jan 2023 14:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 06:06:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

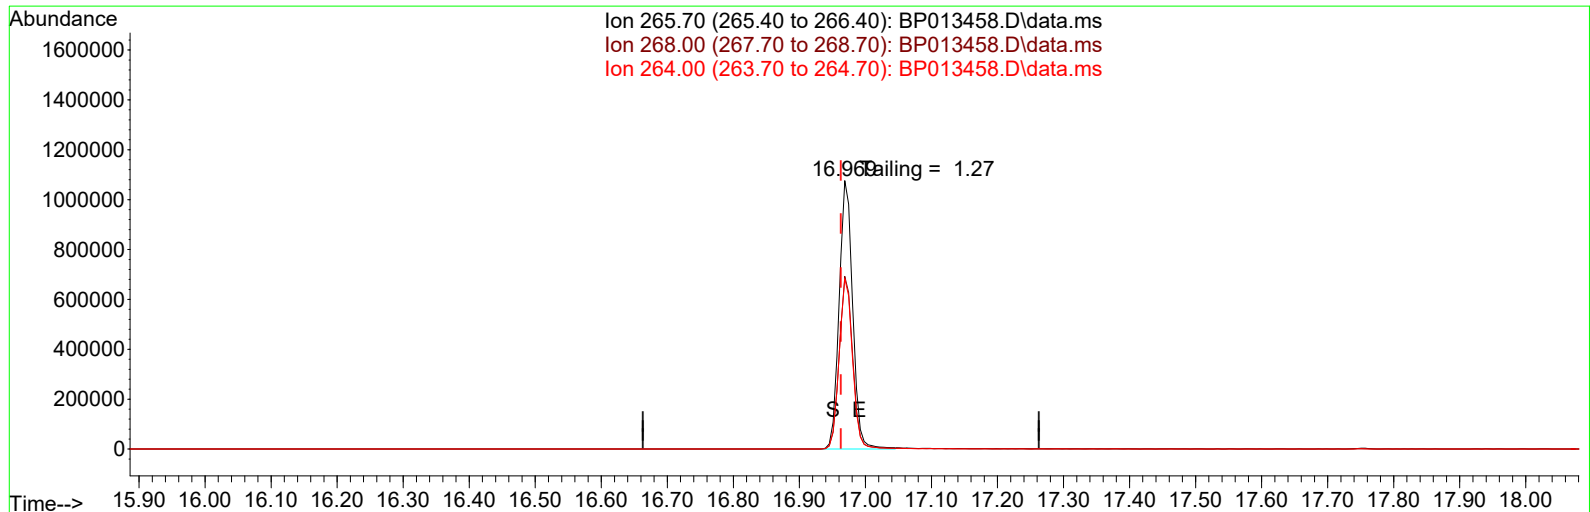

TIC: BP013458.D\data.ms

(70) Pentachlorophenol (C)




16.969min (+ 0.006) 874541.36 ng

response 1542732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.37
264.00	63.00	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011223\
Data File : BP013458.D
Acq On : 12 Jan 2023 14:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 06:06:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

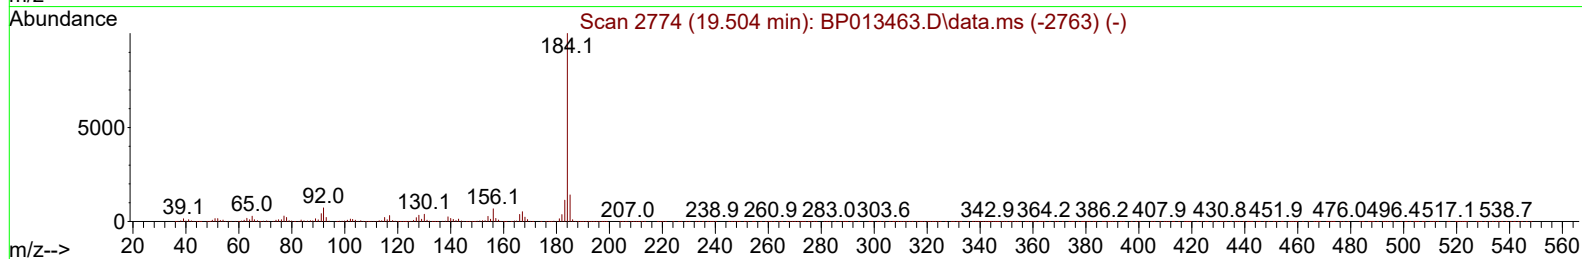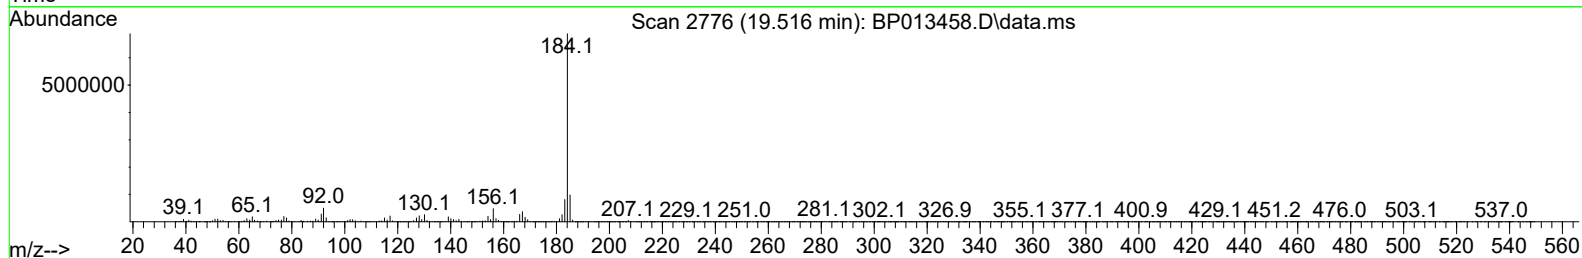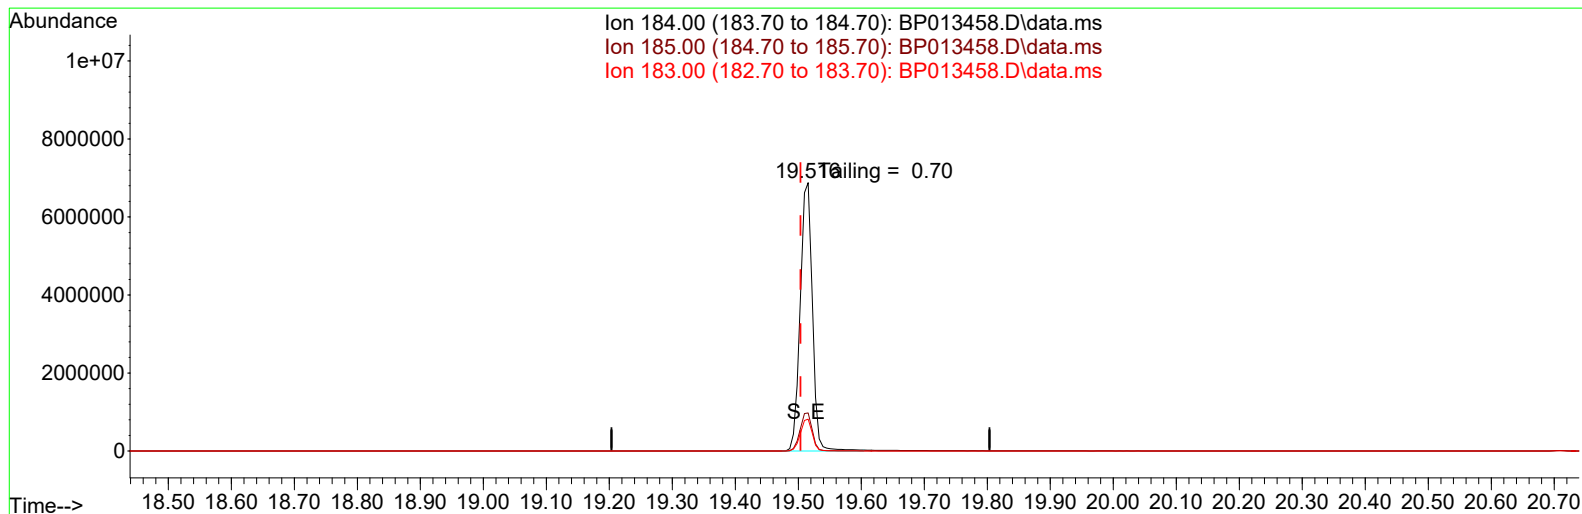

TIC: BP013458.D\data.ms

(77) Benzidine**19.516min (+ 0.012) 380858.68 ng****response 9426919**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.40	11.86
0.00	0.00	0.00