
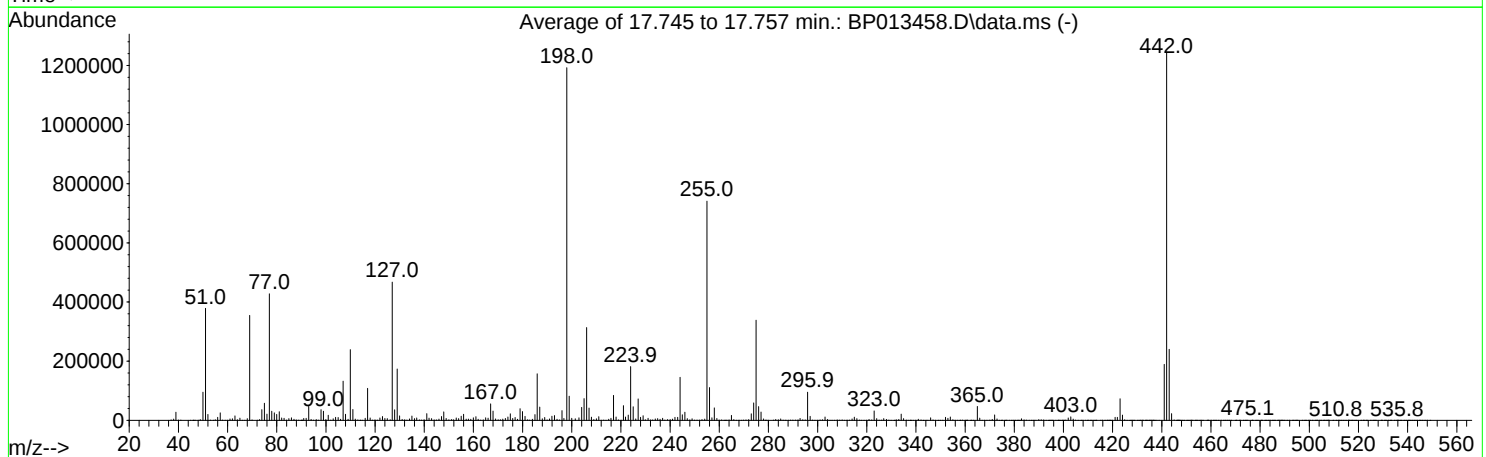


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011223\
Data File : BP013458.D
Acq On : 12 Jan 2023 14:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 13 03:32:57 2023

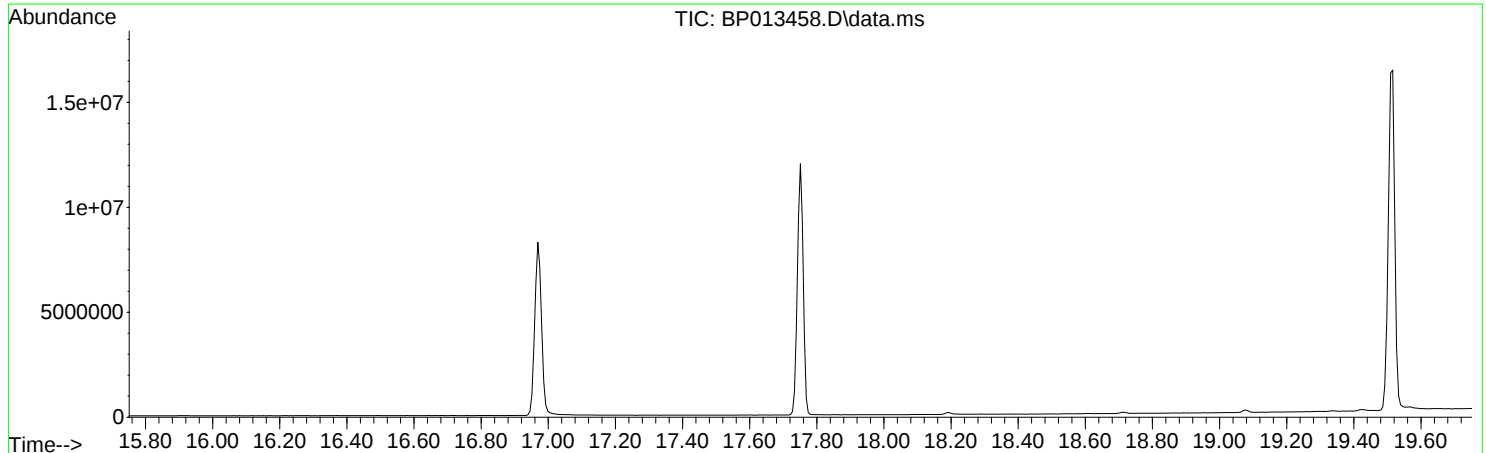




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	378516	PASS
68	69	0.00	2	1.6	5620	PASS
69	198	0.00	100	29.8	354857	PASS
70	69	0.00	2	0.5	1628	PASS
127	198	10	80	39.2	467543	PASS
197	198	0.00	2	0.5	6351	PASS
198	198	100	100	100.0	1192466	PASS
199	198	5	9	6.8	81336	PASS
275	198	10	60	28.4	338603	PASS
365	198	1	100	3.9	46832	PASS
441	198	0.01	100	15.9	189227	PASS
442	442	100	100	100.0	1244075	PASS
443	442	15	24	19.3	240277	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011223\
 Data File : BP013458.D
 Acq On : 12 Jan 2023 14:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 06:06:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 13 03:32:57 2023
 Response via : Initial Calibration

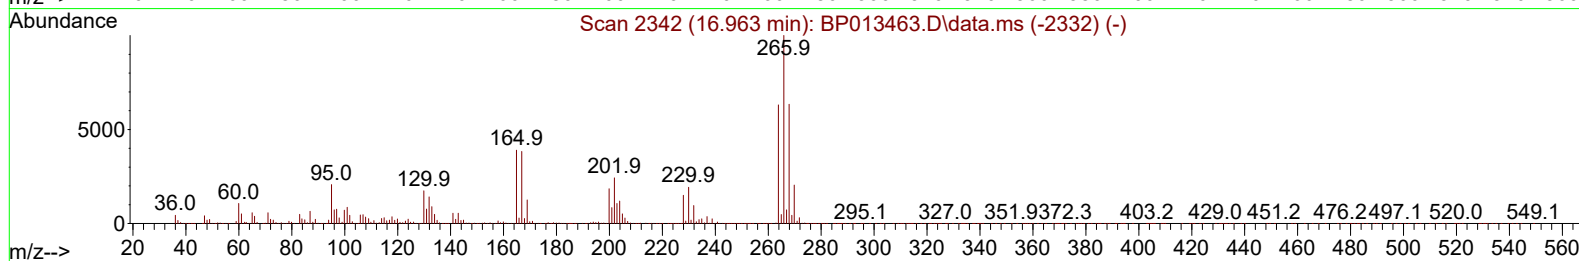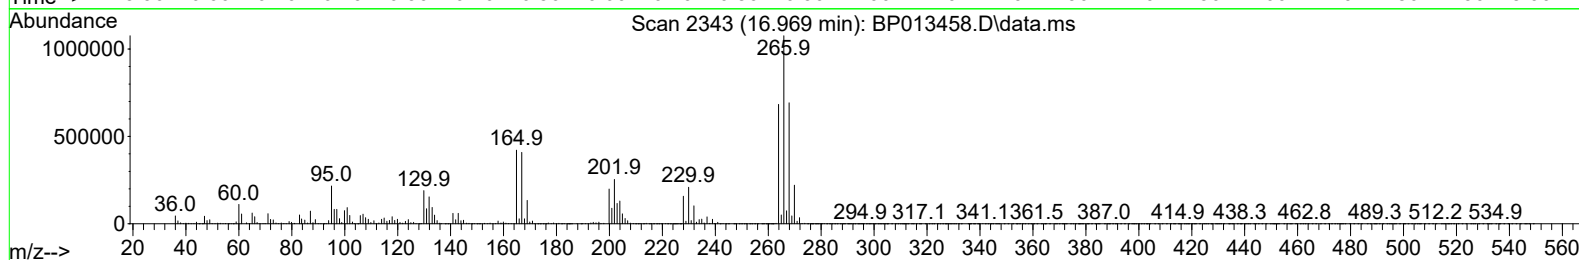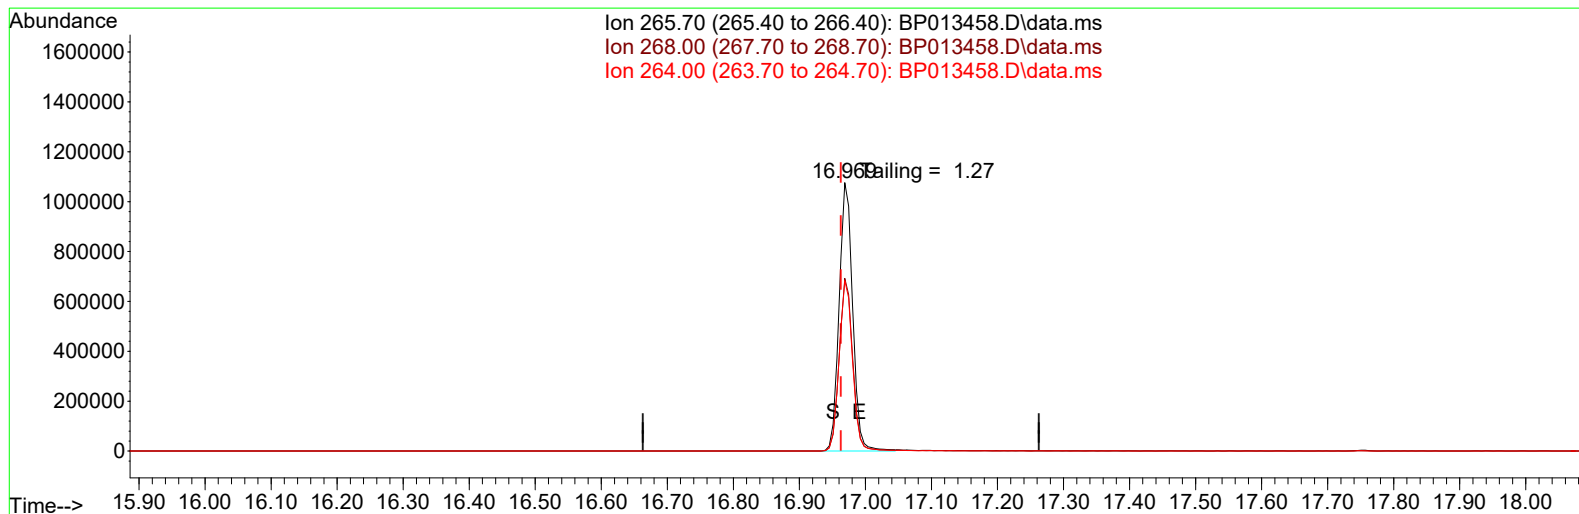

TIC: BP013458.D\data.ms

(70) Pentachlorophenol (C)

16.969min (+ 0.006) 874541.36 ng




response 1542732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.37
264.00	63.00	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011223\
Data File : BP013458.D
Acq On : 12 Jan 2023 14:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 13 06:06:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

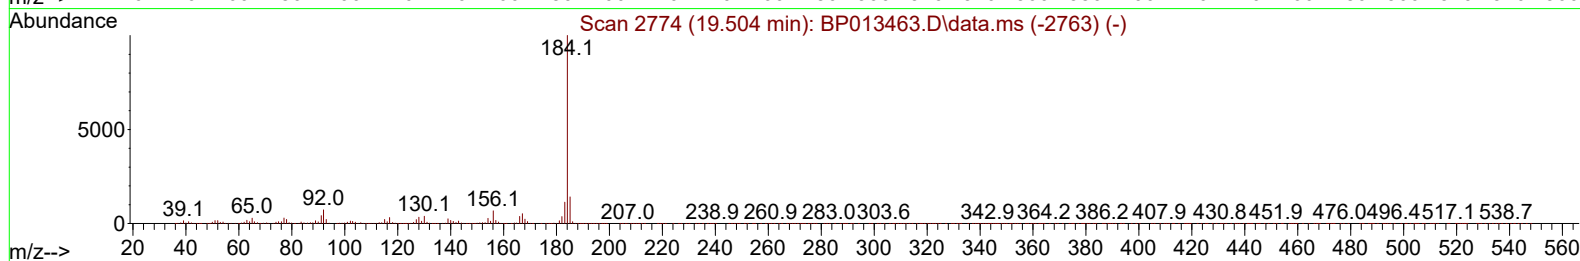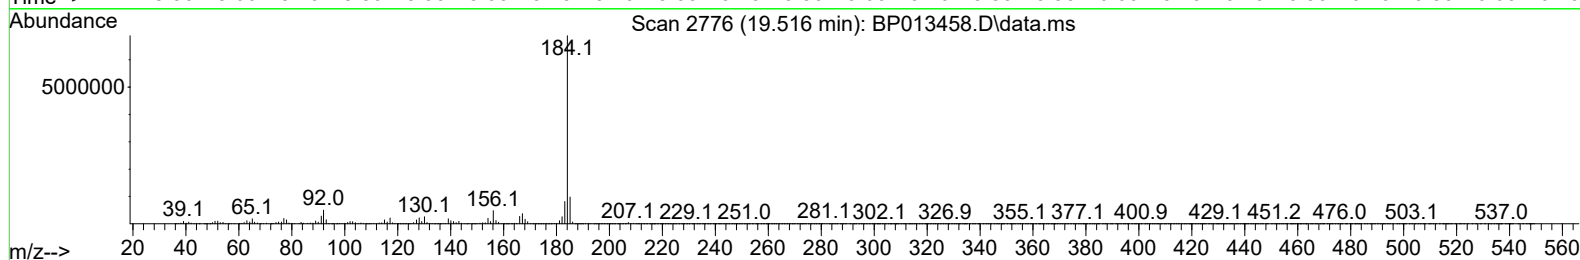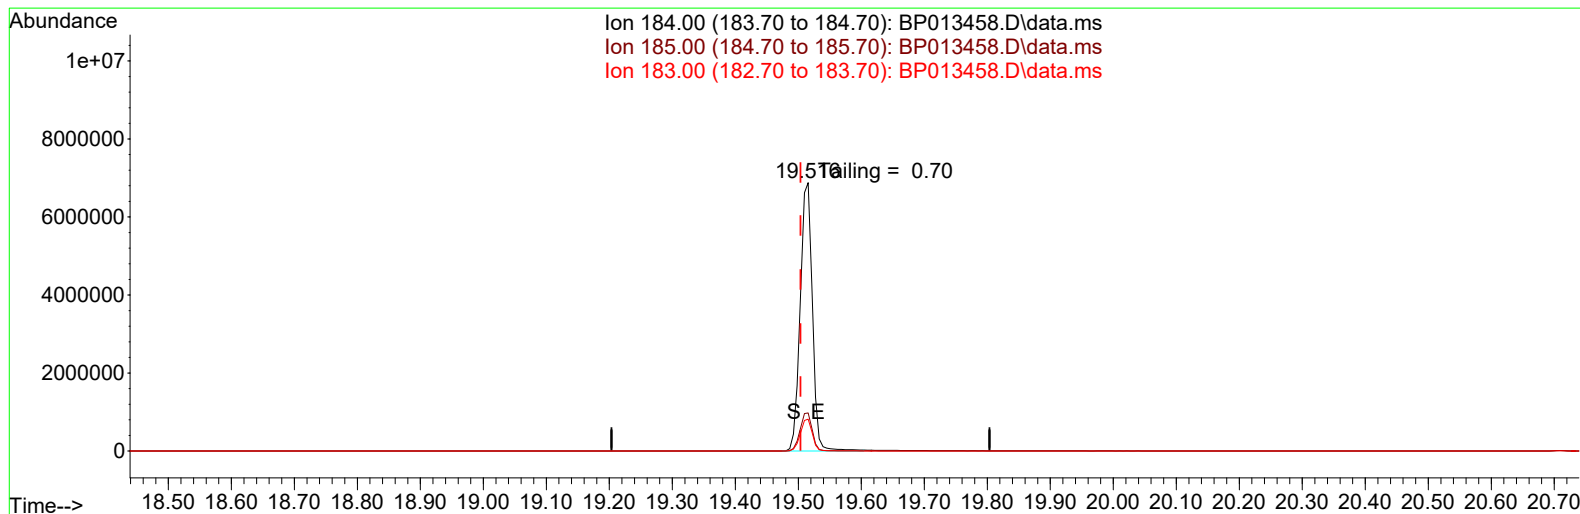

TIC: BP013458.D\data.ms

(77) Benzidine

19.516min (+ 0.012) 380858.68 ng

response 9426919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.40	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2023	BNA_P	<u>BP013458.D</u>
Compound Name	Response	Retention Time
DDT	4353807	20.71
DDD	48020	20.327
DDE	1174	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49194	4403001	1.12

Instrument :
BNA_P
ClientSampleId :
DFTPP