

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019340.D
 Acq On : 12 Jan 2024 20:56
 Operator : MA/JU
 Sample : P1091-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY4

Quant Time: Jan 12 21:38:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 03:05:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	118517	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	488318	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	342139	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	863514	20.000	ng/u1	0.00
79) Chrysene-d12	21.286	240	877868	20.000	ng/u1	0.00
88) Perylene-d12	23.639	264	903147	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.216	96	13451	4.292	ng/uL	0.00
4) Pyridine-d5	3.640	84	92998	10.261	ng/u1	0.00
7) Phenol-d5	6.969	99	80628	7.118	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	244754	36.124	ng/u1	0.00
11) 2-Chlorophenol-d4	7.310	132	217143	27.906	ng/u1	0.00
15) 4-Methylphenol-d8	8.504	113	158665	17.656	ng/u1	-0.01
21) Nitrobenzene-d5	8.945	128	149198	36.317	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	175285	36.721	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	323080	33.502	ng/u1	0.00
31) 4-Chloroaniline-d4	10.728	131	325863	26.750	ng/u1	0.00
46) Dimethylphthalate-d6	13.845	166	1172237	38.781	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	1190938	36.755	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	36366	7.835	ng/u1	0.00
60) Fluorene-d10	15.422	176	999753	40.398	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	236403	37.082	ng/u1	0.00
73) Anthracene-d10	17.280	188	1763350	40.944	ng/u1	0.00
81) Pyrene-d10	19.527	212	2297024	40.128	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.486	264	2095011	42.661	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.252	88	13937	4.293	ng/uL	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019340.D
Acq On : 12 Jan 2024 20:56
Operator : MA/JU
Sample : P1091-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY4

Quant Time: Jan 12 21:38:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 09 03:05:24 2024
Response via : Initial Calibration

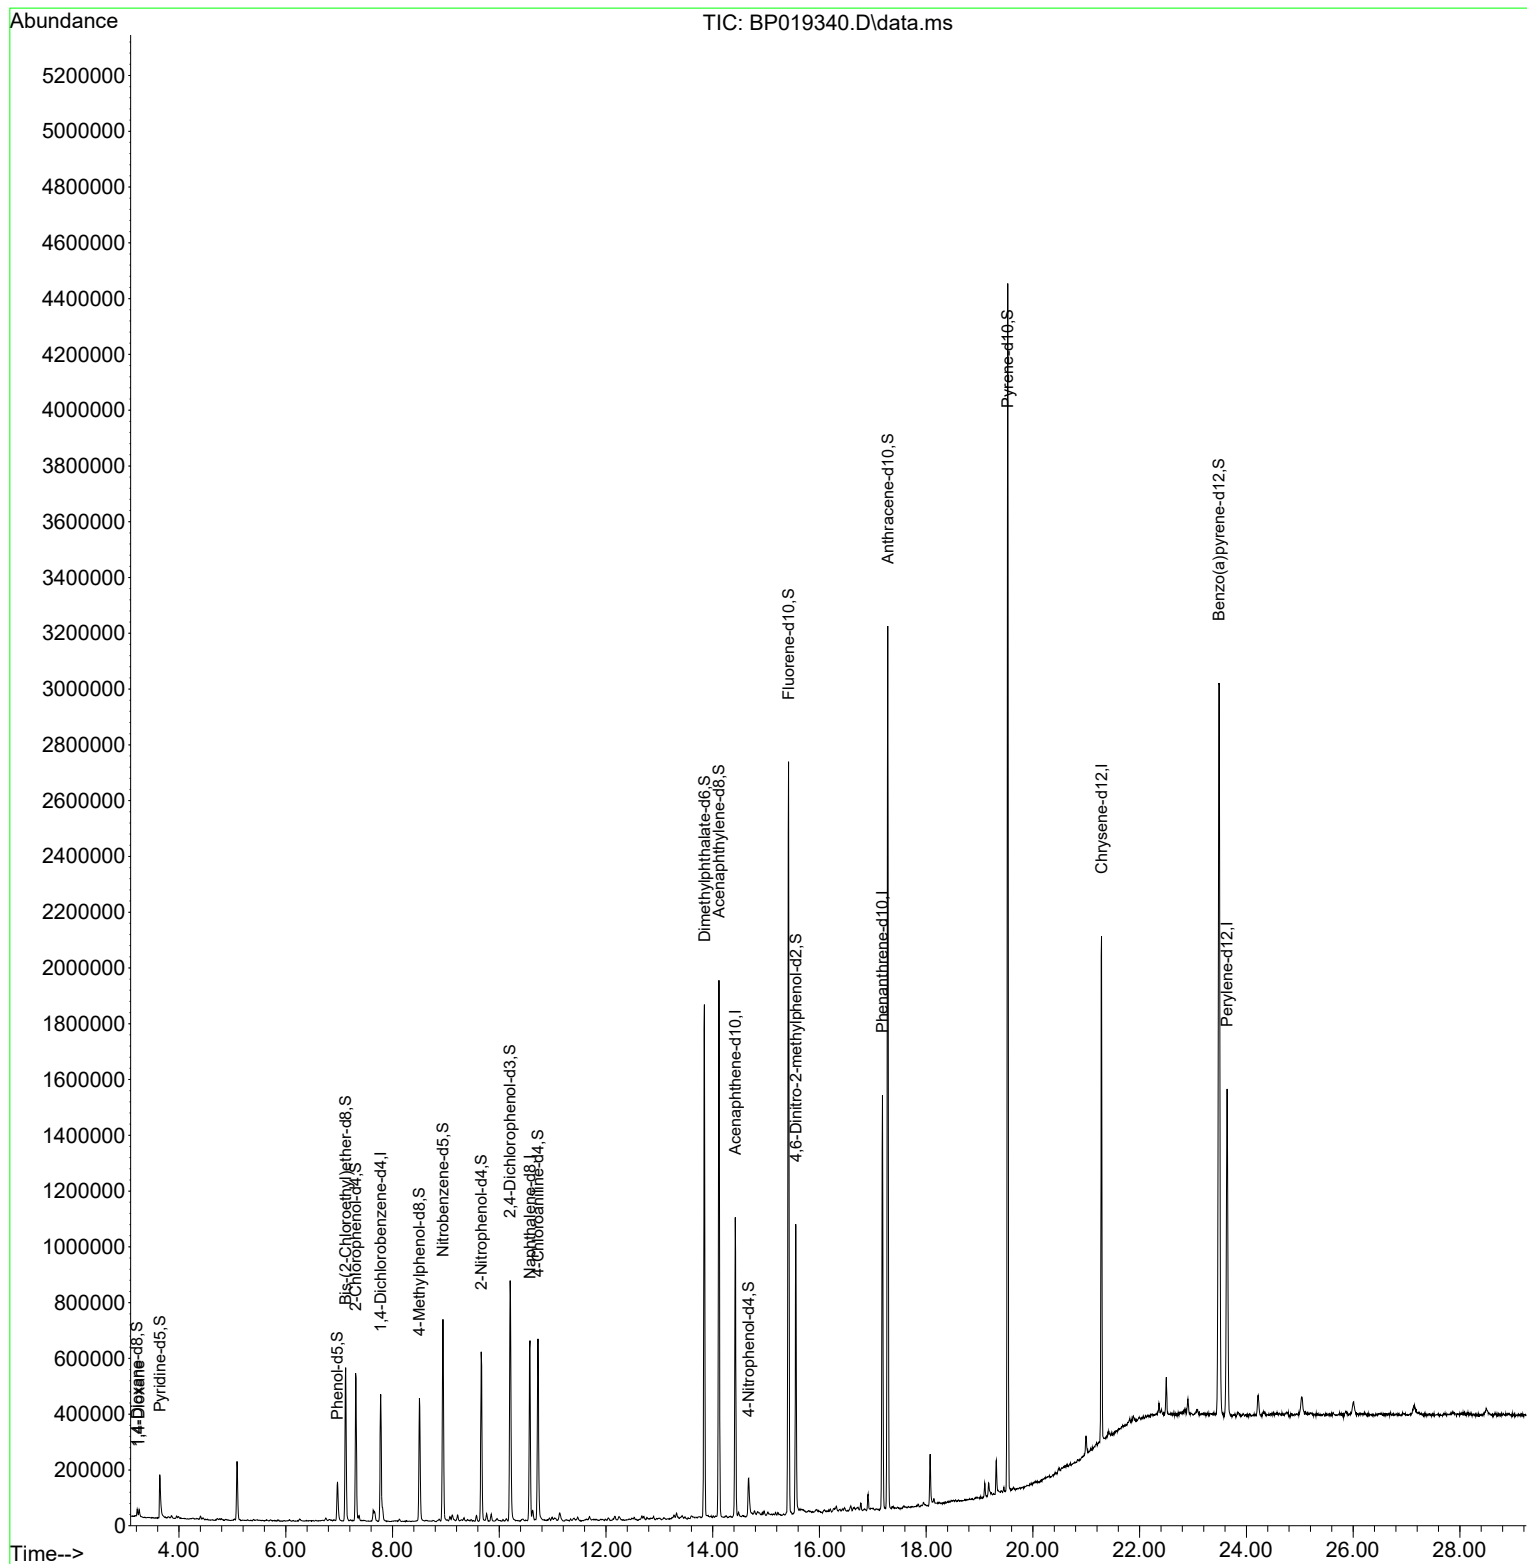

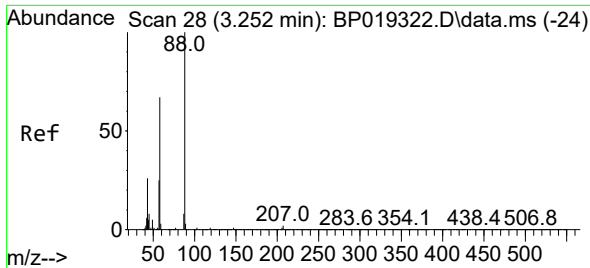

#2
1,4-Dioxane
Concen: 4.293 ng/uL
RT: 3.252 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP019340.D
Acq: 12 Jan 2024 20:56

Instrument :
BNA_P
ClientSampleId :
C0AY4

Tgt Ion: 88 Resp: 13937
Ion Ratio Lower Upper
88 100
43 28.1 22.0 33.0
58 63.4 54.6 82.0

