

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019323.D
 Acq On : 12 Jan 2024 09:48
 Operator : MA/JU
 Sample : PB158377BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	30	rVB	35879	50493	1.27%	0.138%
2	3.634	89	93	113	rBV	469988	758530	19.06%	2.069%
3	3.952	144	147	152	rVB	9945	13075	0.33%	0.036%
4	4.740	279	281	288	rVB7	2359	3993	0.10%	0.011%
5	6.963	652	659	677	rVB	525213	841811	21.15%	2.297%
6	7.116	679	685	696	rVB	414094	645406	16.21%	1.761%
7	7.310	708	718	727	rBV	509766	799059	20.07%	2.180%
8	7.775	789	797	807	rBV	409288	641391	16.11%	1.750%
9	8.504	914	921	941	rBV	649586	1048948	26.35%	2.862%
10	8.946	988	996	1010	rBV	535965	861551	21.64%	2.350%
11	9.663	1107	1118	1133	rBV	460439	748291	18.80%	2.041%
12	10.204	1203	1210	1235	rBV	627697	1136833	28.56%	3.101%
13	10.575	1265	1273	1287	rBV	560729	934996	23.49%	2.551%
14	10.728	1291	1299	1317	rBV	618126	1123001	28.21%	3.064%
15	12.181	1540	1546	1553	rBV	9328	16114	0.40%	0.044%
16	12.757	1641	1644	1652	rVB10	3711	7952	0.20%	0.022%
17	13.322	1735	1740	1745	rBV6	7201	12394	0.31%	0.034%
18	13.698	1794	1804	1805	rBV9	2849	5799	0.15%	0.016%
19	13.845	1816	1829	1841	rBV	1451342	1931038	48.51%	5.268%
20	14.122	1869	1876	1887	rBV	1406855	2086283	52.41%	5.692%
21	14.428	1921	1928	1936	rBV	994862	1428991	35.90%	3.898%
22	14.663	1962	1968	1990	rBV	533664	932058	23.41%	2.543%
23	15.422	2087	2097	2105	rBV	1995931	2776843	69.76%	7.576%
24	15.563	2115	2121	2133	rBV	671242	924242	23.22%	2.521%
25	15.669	2134	2139	2144	rVB3	9273	14609	0.37%	0.040%
26	15.992	2188	2194	2195	rBV5	2450	4060	0.10%	0.011%
27	16.210	2226	2231	2236	rVB4	8752	13964	0.35%	0.038%
28	16.651	2302	2306	2310	rVB5	3481	5617	0.14%	0.015%
29	16.857	2334	2341	2348	rBV5	6624	14653	0.37%	0.040%
30	16.969	2357	2360	2362	rBV4	3507	3994	0.10%	0.011%
31	17.186	2390	2397	2405	rBV	1394921	1941794	48.78%	5.297%
32	17.286	2407	2414	2427	rVB	2264102	3174140	79.74%	8.659%
33	18.080	2546	2549	2555	rBV7	9098	14406	0.36%	0.039%
34	19.104	2719	2723	2728	rBV2	34381	50408	1.27%	0.138%
35	19.174	2732	2735	2740	rVV	25456	35157	0.88%	0.096%
36	19.533	2790	2796	2803	rBV	2994510	3980708	100.00%	10.860%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019323.D
Acq On : 12 Jan 2024 09:48
Operator : MA/JU
Sample : PB158377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK377

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	21.292	3090	3095	3104	rVB	1678690	2146827	53.93%	5.857%
38	23.498	3463	3470	3479	rVB2	1793016	3519034	88.40%	9.600%
39	23.645	3489	3495	3507	rVB	1010653	2006752	50.41%	5.475%




Sum of corrected areas: 36655215

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019323.D
Acq On : 12 Jan 2024 09:48
Operator : MA/JU
Sample : PB158377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

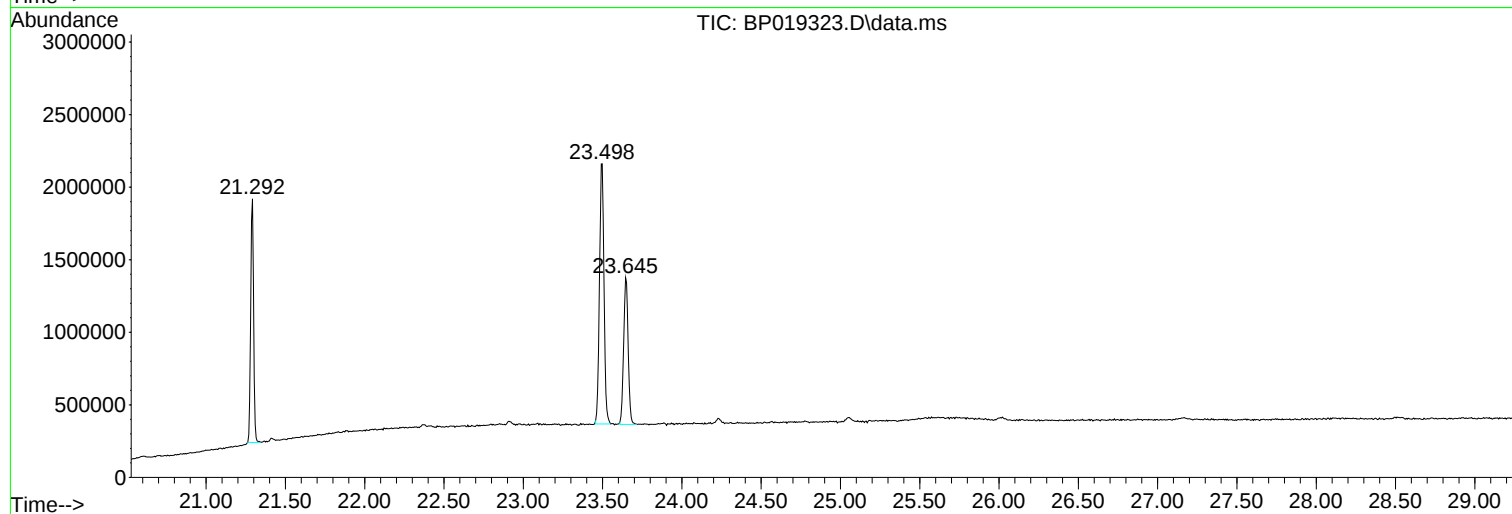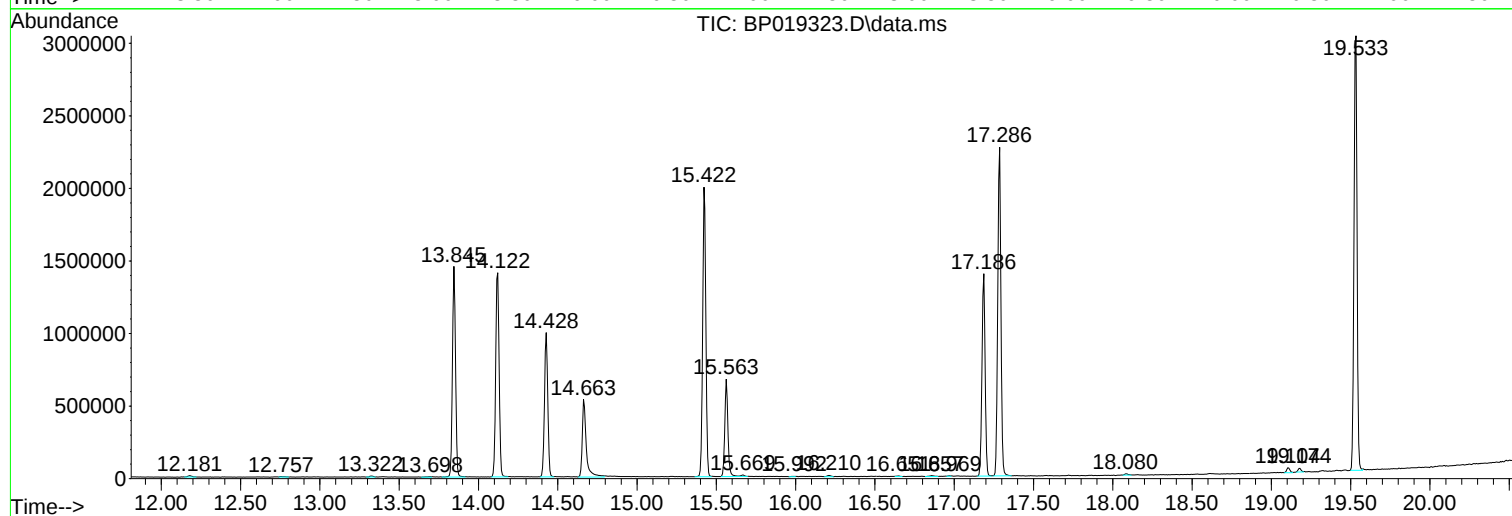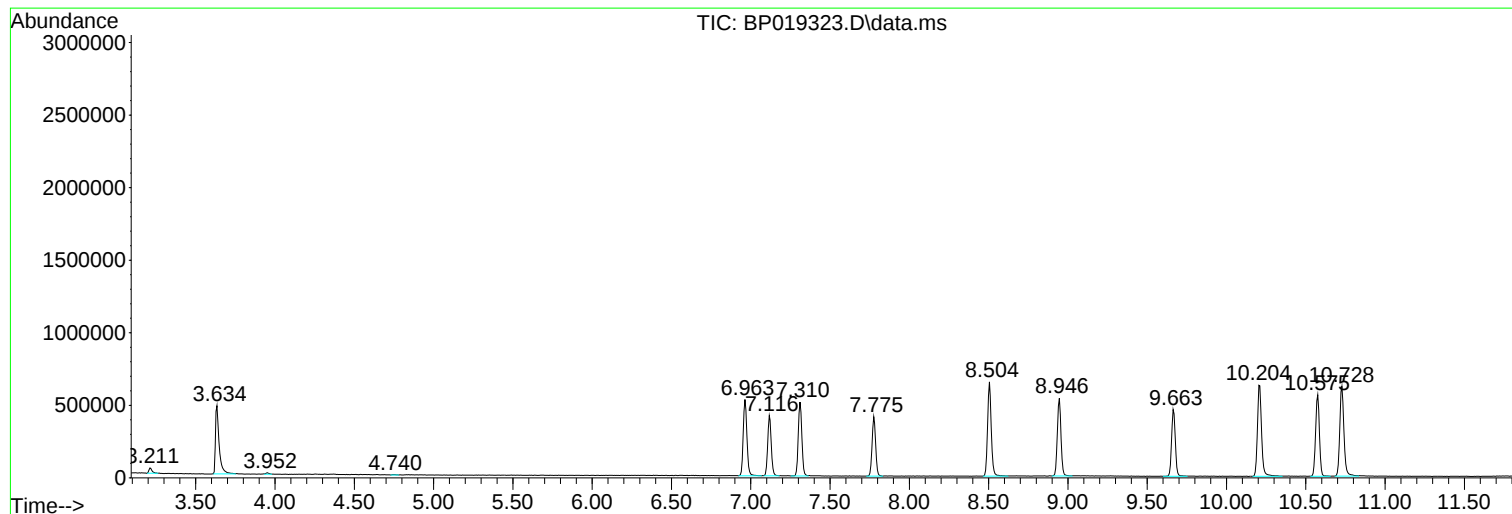

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019323.D
Acq On : 12 Jan 2024 09:48
Operator : MA/JU
Sample : PB158377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019323.D
Acq On : 12 Jan 2024 09:48
Operator : MA/JU
Sample : PB158377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc