

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019331.D
 Acq On : 12 Jan 2024 15:49
 Operator : MA/JU
 Sample : PB158381BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK381

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	28	rBV	31220	44998	1.13%	0.118%
2	3.634	89	93	114	rBV	414643	701265	17.61%	1.845%
3	3.958	144	148	152	rVB2	7108	9812	0.25%	0.026%
4	6.969	653	660	670	rBV	513817	837374	21.03%	2.203%
5	7.122	679	686	697	rBV	414095	649858	16.32%	1.710%
6	7.316	711	719	728	rBV	492780	809570	20.33%	2.130%
7	7.781	791	798	807	rBV	470173	747516	18.77%	1.967%
8	8.505	915	921	935	rBV	634235	1063060	26.69%	2.797%
9	8.946	989	996	1009	rBV	543673	865793	21.74%	2.278%
10	9.663	1112	1118	1135	rBV	440366	753784	18.93%	1.984%
11	10.210	1204	1211	1232	rBV	641366	1153527	28.96%	3.035%
12	10.575	1265	1273	1281	rBV	666112	1079274	27.10%	2.840%
13	10.728	1291	1299	1314	rBV	621764	1127577	28.31%	2.967%
14	12.181	1540	1546	1554	rBV6	8778	17384	0.44%	0.046%
15	13.328	1735	1741	1745	rBV3	12302	20874	0.52%	0.055%
16	13.404	1749	1754	1757	rBV7	2538	4020	0.10%	0.011%
17	13.845	1822	1829	1841	rBV	1323103	1837062	46.13%	4.834%
18	14.116	1868	1875	1886	rBV	1408199	2025861	50.87%	5.331%
19	14.422	1920	1927	1936	rBV	1078846	1585811	39.82%	4.173%
20	14.663	1962	1968	1985	rBV	504440	909593	22.84%	2.394%
21	15.422	2087	2097	2104	rBV	1912866	2688435	67.51%	7.074%
22	15.557	2114	2120	2133	rBV	631023	926939	23.28%	2.439%
23	15.663	2134	2138	2143	rVB3	8884	13261	0.33%	0.035%
24	16.210	2225	2231	2235	rBV5	8046	12321	0.31%	0.032%
25	16.857	2337	2341	2351	rVB10	5178	10827	0.27%	0.028%
26	16.963	2357	2359	2365	rBV4	3780	5108	0.13%	0.013%
27	17.181	2389	2396	2405	rBV	1594152	2199035	55.22%	5.787%
28	17.281	2406	2413	2426	rVB	2243545	3138431	78.81%	8.259%
29	17.951	2523	2527	2532	rBV7	3066	6387	0.16%	0.017%
30	18.075	2545	2548	2553	rBV6	11523	16034	0.40%	0.042%
31	19.098	2718	2722	2727	rBV2	33988	49167	1.23%	0.129%
32	19.175	2731	2735	2740	rVV	25168	36850	0.93%	0.097%
33	19.528	2789	2795	2806	rBV	3000234	3982518	100.00%	10.480%
34	21.286	3089	3094	3100	rVB	1991780	2546857	63.95%	6.702%
35	23.486	3461	3468	3479	rVB	1987283	3740975	93.93%	9.844%
36	23.639	3487	3494	3502	rVB	1226931	2385258	59.89%	6.277%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019331.D
Acq On : 12 Jan 2024 15:49
Operator : MA/JU
Sample : PB158381BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK381

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 38002416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019331.D
Acq On : 12 Jan 2024 15:49
Operator : MA/JU
Sample : PB158381BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

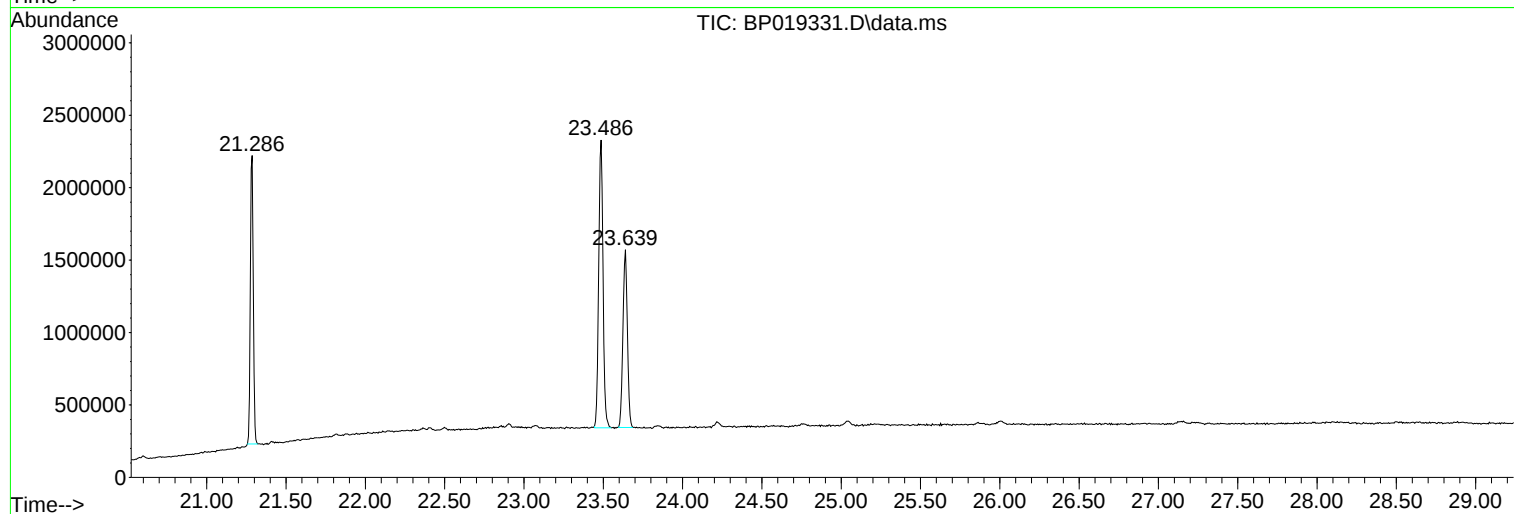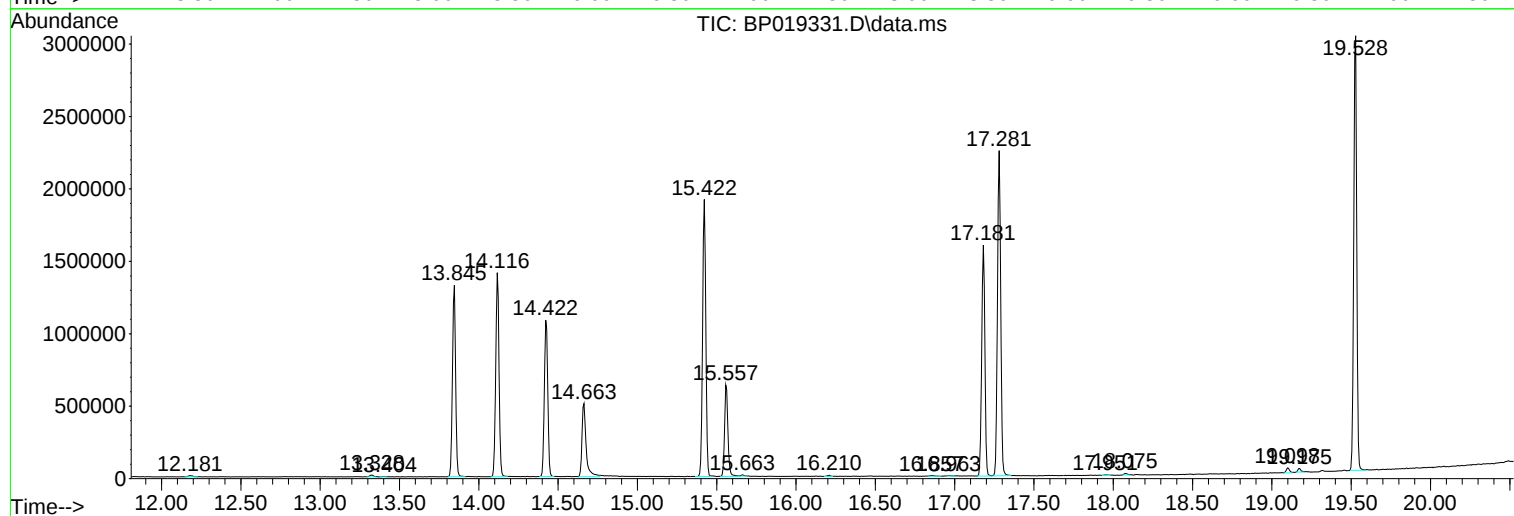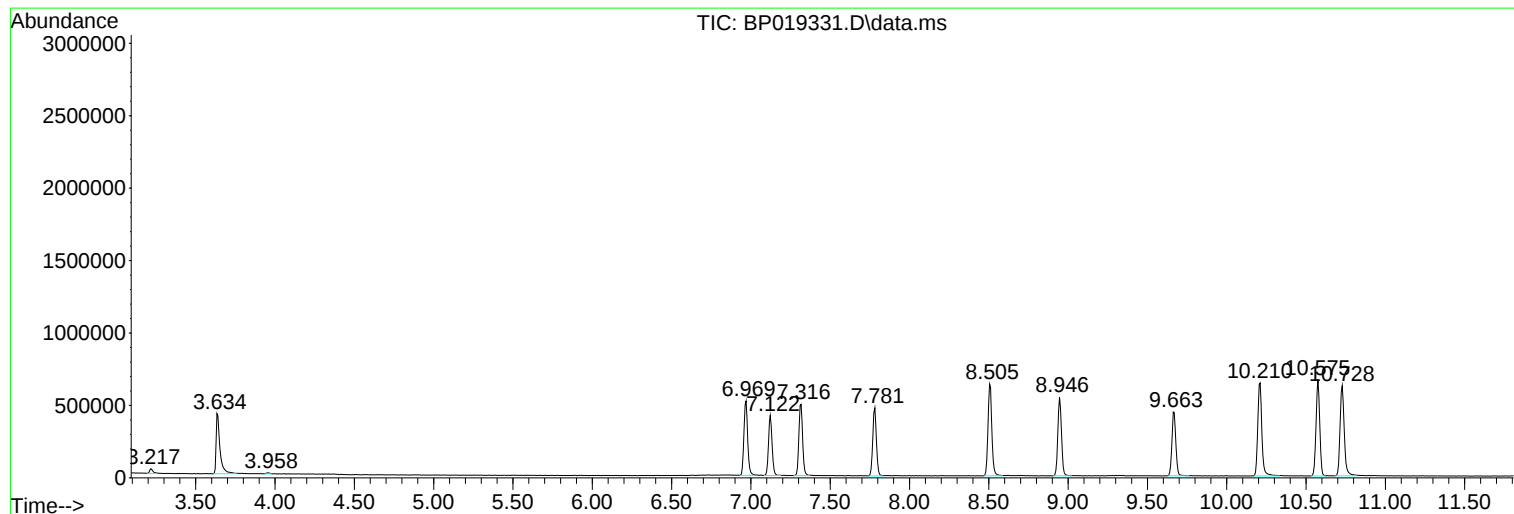

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019331.D
Acq On : 12 Jan 2024 15:49
Operator : MA/JU
Sample : PB158381BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019331.D
Acq On : 12 Jan 2024 15:49
Operator : MA/JU
Sample : PB158381BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc