

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019332.D
 Acq On : 12 Jan 2024 16:23
 Operator : MA/JU
 Sample : PB158382BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK382

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	34	rVB	32309	49560	1.28%	0.134%
2	3.634	90	93	115	rBV	411473	697069	17.94%	1.878%
3	3.958	145	148	155	rVB3	7751	14265	0.37%	0.038%
4	6.969	653	660	670	rBV	508545	830788	21.38%	2.238%
5	7.122	680	686	695	rBV	415769	635666	16.36%	1.713%
6	7.316	712	719	729	rBV	490820	795298	20.47%	2.143%
7	7.781	791	798	808	rBV	444789	706879	18.19%	1.904%
8	8.504	913	921	935	rBV	631197	1052844	27.09%	2.836%
9	8.946	986	996	1006	rBV	528679	866537	22.30%	2.335%
10	9.669	1111	1119	1128	rBV	446026	746647	19.21%	2.012%
11	10.210	1202	1211	1230	rBV	637672	1146248	29.50%	3.088%
12	10.575	1264	1273	1282	rBV	624454	1024842	26.37%	2.761%
13	10.728	1291	1299	1315	rBV	604403	1121509	28.86%	3.021%
14	12.175	1539	1545	1553	rBV4	9867	22336	0.57%	0.060%
15	13.322	1734	1740	1745	rBV6	8182	13981	0.36%	0.038%
16	13.845	1822	1829	1839	rBV	1303147	1820829	46.85%	4.905%
17	14.116	1867	1875	1887	rBV	1365665	1995464	51.35%	5.376%
18	14.422	1920	1927	1937	rBV	1022711	1499471	38.59%	4.040%
19	14.663	1961	1968	1993	rBV	516844	920618	23.69%	2.480%
20	15.422	2090	2097	2104	rBV	1840436	2634071	67.78%	7.096%
21	15.557	2113	2120	2134	rBV	644675	935825	24.08%	2.521%
22	15.663	2134	2138	2143	rVB3	8501	14376	0.37%	0.039%
23	16.204	2226	2230	2237	rVB9	6830	10868	0.28%	0.029%
24	16.863	2337	2342	2347	rVB9	4448	6960	0.18%	0.019%
25	16.975	2355	2361	2365	rBV3	4046	7072	0.18%	0.019%
26	17.180	2390	2396	2406	rBV	1545057	2063005	53.09%	5.558%
27	17.280	2406	2413	2431	rVB	2191740	3107397	79.96%	8.372%
28	18.086	2546	2550	2554	rBV7	4293	7485	0.19%	0.020%
29	18.145	2558	2560	2564	rBV5	3595	4458	0.11%	0.012%
30	19.104	2718	2723	2727	rBV	33403	45871	1.18%	0.124%
31	19.175	2731	2735	2740	rVV	26278	35982	0.93%	0.097%
32	19.527	2789	2795	2804	rBV	2986884	3886127	100.00%	10.470%
33	21.286	3089	3094	3102	rBV	1942906	2394271	61.61%	6.450%
34	23.486	3461	3468	3482	rVB	1934670	3722055	95.78%	10.028%
35	23.639	3488	3494	3506	rVB	1125651	2281504	58.71%	6.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019332.D
Acq On : 12 Jan 2024 16:23
Operator : MA/JU
Sample : PB158382BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK382

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 37118178

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019332.D
Acq On : 12 Jan 2024 16:23
Operator : MA/JU
Sample : PB158382BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK382

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

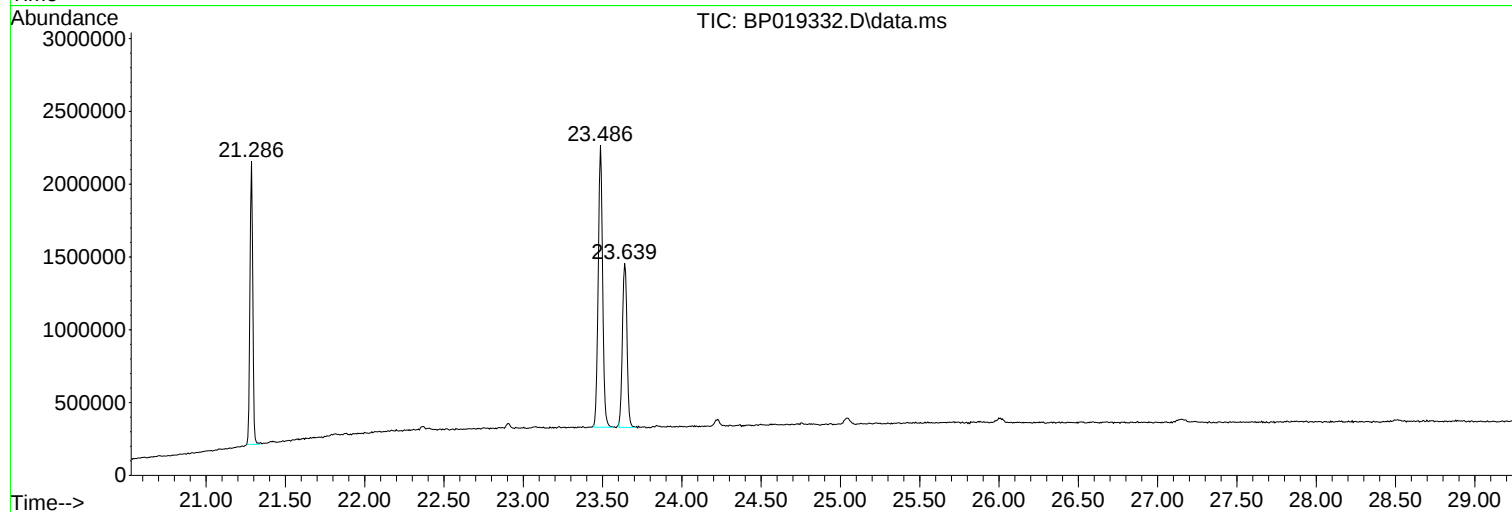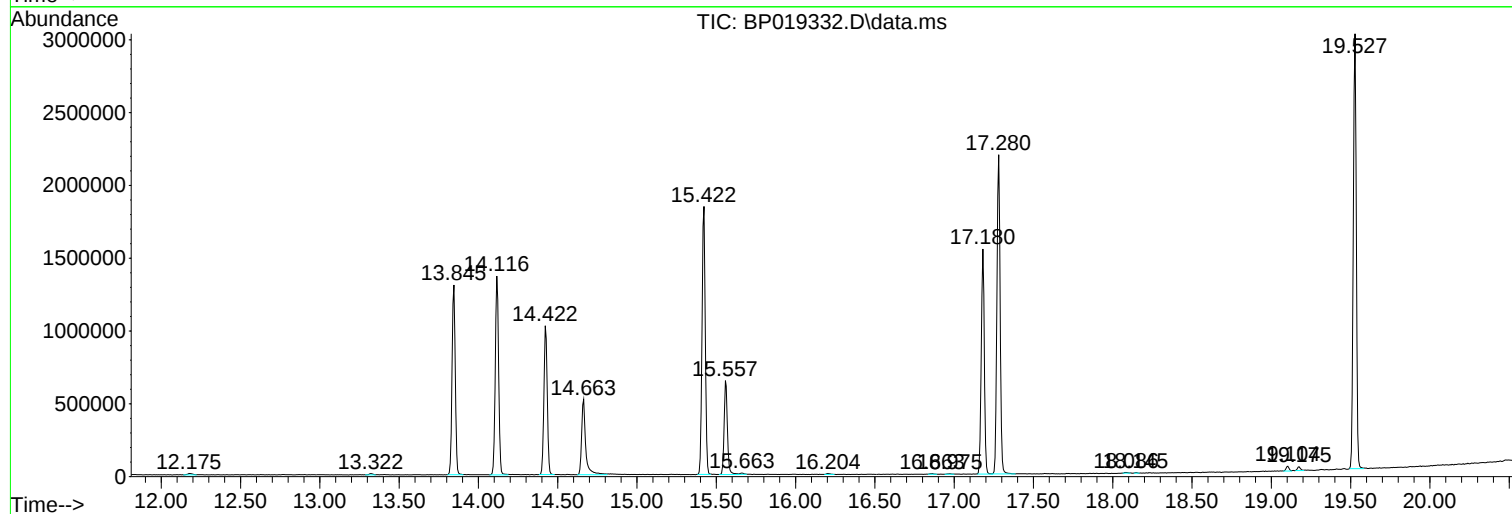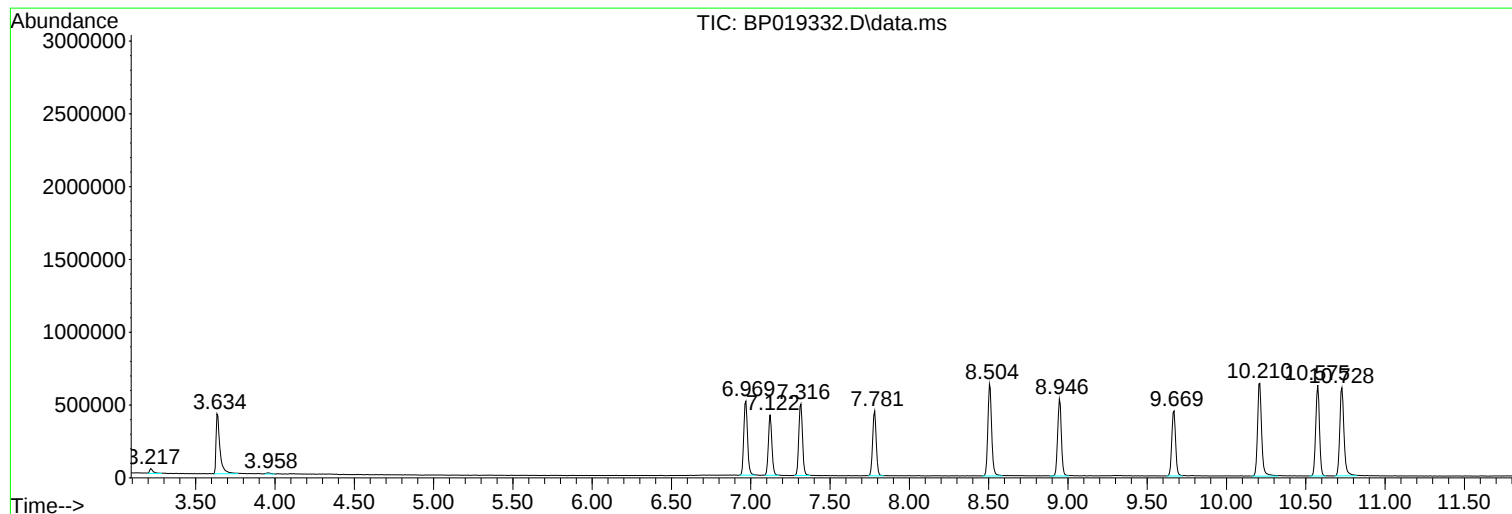

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019332.D
Acq On : 12 Jan 2024 16:23
Operator : MA/JU
Sample : PB158382BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK382

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019332.D
Acq On : 12 Jan 2024 16:23
Operator : MA/JU
Sample : PB158382BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK382

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc