

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019334.D
 Acq On : 12 Jan 2024 17:32
 Operator : MA/JU
 Sample : P1091-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	30	rVB	19664	27795	0.80%	0.090%
2	3.646	91	95	107	rBV	106006	189178	5.45%	0.613%
3	3.958	144	148	154	rVB2	7143	10659	0.31%	0.035%
4	6.969	653	660	668	rBV	70378	124937	3.60%	0.405%
5	7.122	679	686	700	rVB	330376	528128	15.21%	1.710%
6	7.316	712	719	730	rBV	276345	462799	13.32%	1.499%
7	7.781	789	798	807	rBV	465075	762894	21.96%	2.471%
8	8.510	915	922	932	rBV	208197	366163	10.54%	1.186%
9	8.946	989	996	1008	rBV	414521	688196	19.81%	2.229%
10	9.334	1059	1062	1069	rVB9	4449	8618	0.25%	0.028%
11	9.663	1111	1118	1131	rBV	306064	520061	14.97%	1.684%
12	10.210	1204	1211	1230	rBV	415062	764720	22.02%	2.477%
13	10.575	1263	1273	1280	rBV	630719	1060162	30.52%	3.434%
14	10.622	1280	1281	1289	rVB7	2230	3735	0.11%	0.012%
15	10.728	1292	1299	1317	rVV	377234	707562	20.37%	2.292%
16	10.898	1325	1328	1334	rVB8	2341	4810	0.14%	0.016%
17	11.410	1411	1415	1419	rBV6	2271	3615	0.10%	0.012%
18	12.004	1511	1516	1524	rVB6	3679	6990	0.20%	0.023%
19	12.181	1540	1546	1551	rBV2	7954	15895	0.46%	0.051%
20	13.239	1721	1726	1733	rVV3	6857	8984	0.26%	0.029%
21	13.322	1735	1740	1744	rVV3	9417	13852	0.40%	0.045%
22	13.398	1748	1753	1761	rVB3	6089	10541	0.30%	0.034%
23	13.845	1820	1829	1838	rBV	1088006	1544786	44.48%	5.003%
24	14.116	1868	1875	1888	rBV	1167245	1673518	48.18%	5.420%
25	14.316	1907	1909	1915	rVB7	2570	3500	0.10%	0.011%
26	14.422	1919	1927	1938	rBV	1099129	1611247	46.39%	5.218%
27	14.686	1965	1972	1985	rBV6	25158	71750	2.07%	0.232%
28	15.222	2060	2063	2068	rVB6	2474	4053	0.12%	0.013%
29	15.422	2089	2097	2108	rBV	1554596	2279242	65.62%	7.382%
30	15.557	2114	2120	2132	rBV	215883	335621	9.66%	1.087%
31	15.663	2134	2138	2144	rVB7	7735	12693	0.37%	0.041%
32	16.045	2201	2203	2208	rBV6	2877	3888	0.11%	0.013%
33	16.204	2226	2230	2236	rBV7	6541	11676	0.34%	0.038%
34	16.322	2246	2250	2254	rVB6	4350	7102	0.20%	0.023%
35	16.569	2289	2292	2294	rBV4	3112	3760	0.11%	0.012%
36	16.592	2294	2296	2302	rVB7	3171	4799	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019334.D
 Acq On : 12 Jan 2024 17:32
 Operator : MA/JU
 Sample : P1091-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	16.857	2338	2341	2344	rBV5	3319	3766	0.11%	0.012%
38	16.910	2345	2350	2357	rBV	143266	191486	5.51%	0.620%
39	16.969	2357	2360	2363	rVV4	2739	3799	0.11%	0.012%
40	17.180	2388	2396	2405	rBV	1574811	2127945	61.27%	6.892%
41	17.280	2406	2413	2424	rVV	1952342	2772108	79.81%	8.978%
42	17.404	2429	2434	2443	rVB4	10179	22254	0.64%	0.072%
43	17.586	2461	2465	2467	rBV5	2710	4373	0.13%	0.014%
44	18.075	2542	2548	2557	rBV	74905	113647	3.27%	0.368%
45	18.486	2614	2618	2621	rBV6	6840	9611	0.28%	0.031%
46	19.098	2719	2722	2729	rVB2	29443	39962	1.15%	0.129%
47	19.174	2731	2735	2742	rBV	26538	51541	1.48%	0.167%
48	19.310	2754	2758	2764	rBV3	45065	66694	1.92%	0.216%
49	19.451	2780	2782	2788	rBV7	14241	18905	0.54%	0.061%
50	19.527	2789	2795	2803	rVV	2637633	3473304	100.00%	11.249%
51	20.992	3041	3044	3049	rBV5	65322	91032	2.62%	0.295%
52	21.286	3088	3094	3101	rBV	1812960	2454614	70.67%	7.950%
53	23.486	3461	3468	3480	rVB	1642933	3282842	94.52%	10.632%
54	23.639	3487	3494	3505	rVB	1154020	2290372	65.94%	7.418%




Sum of corrected areas: 30876184

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019334.D
Acq On : 12 Jan 2024 17:32
Operator : MA/JU
Sample : P1091-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

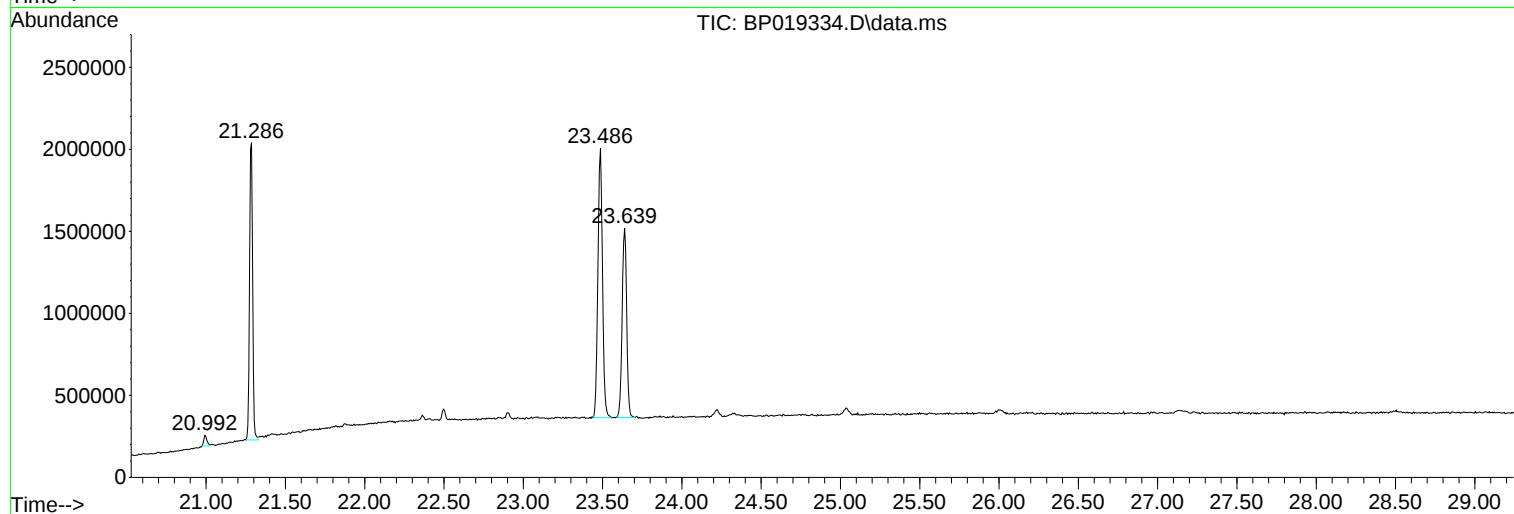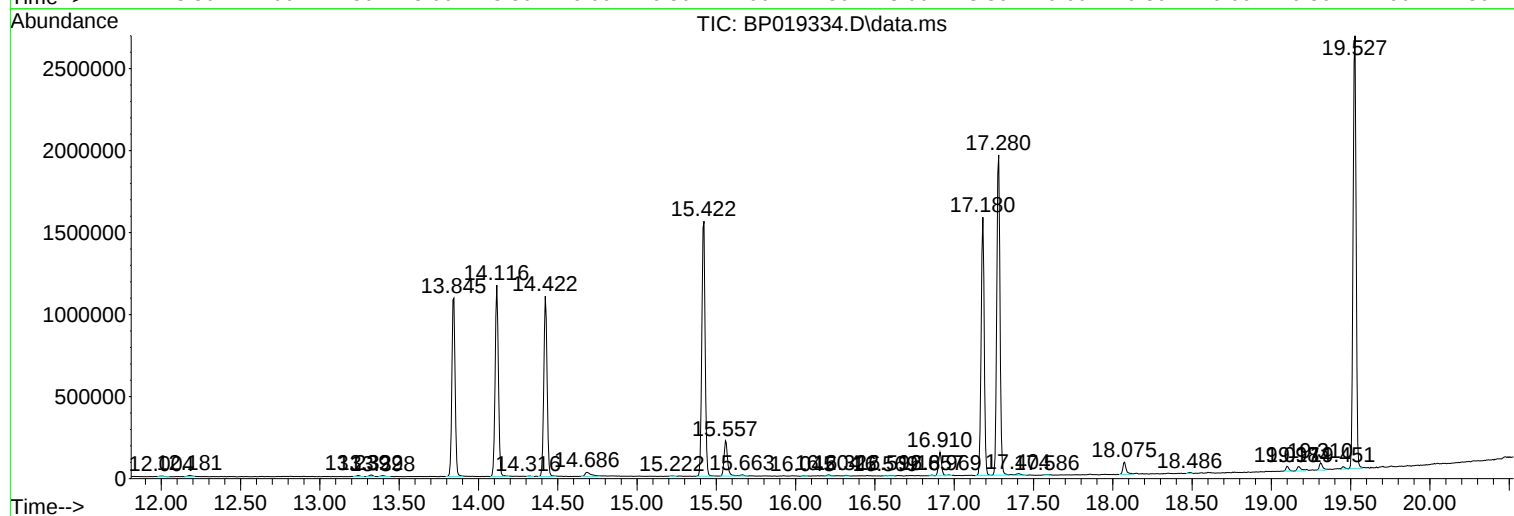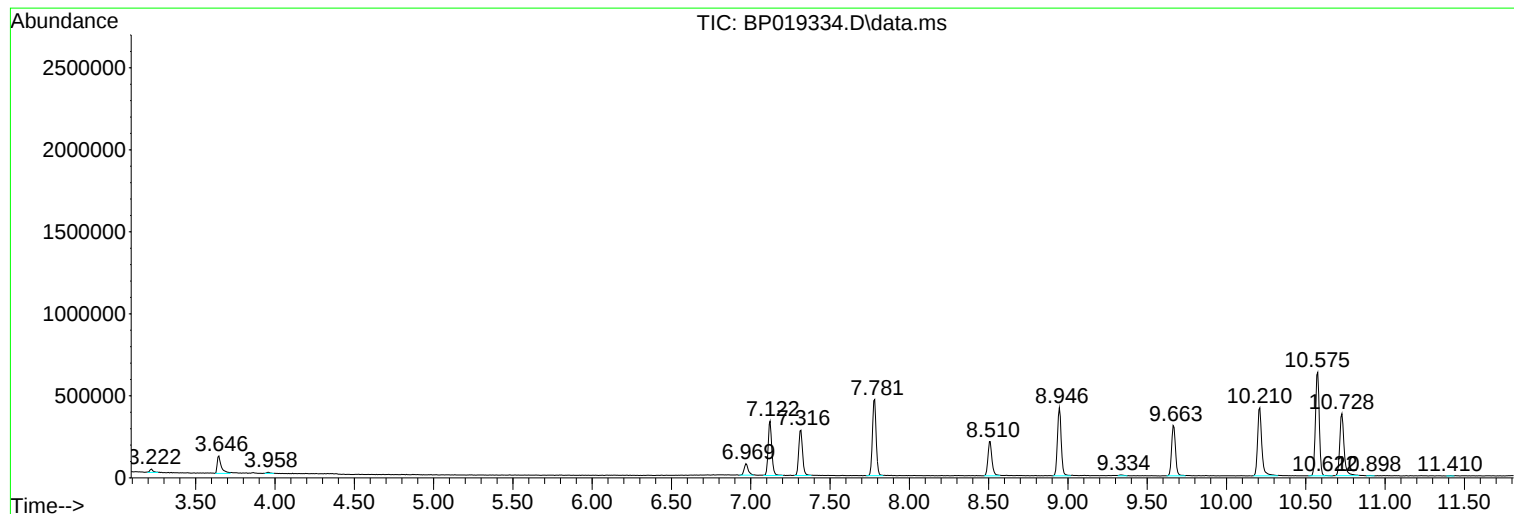

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019334.D
Acq On : 12 Jan 2024 17:32
Operator : MA/JU
Sample : P1091-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019334.D
Acq On : 12 Jan 2024 17:32
Operator : MA/JU
Sample : P1091-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------