

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019338.D
 Acq On : 12 Jan 2024 19:48
 Operator : MA/JU
 Sample : P1091-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	25	rBV	25757	31246	1.26%	0.149%
2	3.252	25	28	35	rVB2	12588	20787	0.84%	0.099%
3	3.640	90	94	112	rBV	129348	223939	9.06%	1.066%
4	3.958	143	148	158	rBV	89153	129201	5.22%	0.615%
5	6.075	505	508	511	rBV5	1886	2658	0.11%	0.013%
6	6.634	600	603	606	rBV5	2372	2983	0.12%	0.014%
7	6.699	610	614	615	rBV4	2313	2648	0.11%	0.013%
8	6.969	654	660	670	rVB	132943	230619	9.33%	1.098%
9	7.122	680	686	694	rBV	163497	255356	10.33%	1.215%
10	7.316	712	719	728	rBV	171079	284222	11.49%	1.353%
11	7.775	791	797	806	rBV	471560	767971	31.06%	3.655%
12	8.511	915	922	932	rBV	174050	310835	12.57%	1.479%
13	8.946	987	996	1007	rBV	200559	341034	13.79%	1.623%
14	9.334	1060	1062	1068	rVB7	2481	3240	0.13%	0.015%
15	9.663	1112	1118	1134	rBV	151154	266834	10.79%	1.270%
16	10.210	1204	1211	1230	rBV	210880	406825	16.45%	1.936%
17	10.575	1264	1273	1282	rBV	659730	1100579	44.51%	5.238%
18	10.728	1292	1299	1313	rBV	173375	337682	13.66%	1.607%
19	11.452	1420	1422	1427	rVB5	2055	2650	0.11%	0.013%
20	12.187	1540	1547	1556	rBV10	3888	10362	0.42%	0.049%
21	12.763	1642	1645	1647	rBV4	2218	2500	0.10%	0.012%
22	13.151	1706	1711	1714	rVB7	1648	2722	0.11%	0.013%
23	13.322	1734	1740	1749	rBV3	13337	24532	0.99%	0.117%
24	13.404	1751	1754	1761	rVB9	2124	4595	0.19%	0.022%
25	13.840	1821	1828	1839	rBV	524261	770419	31.15%	3.666%
26	14.116	1868	1875	1888	rBV2	564608	836062	33.81%	3.979%
27	14.422	1920	1927	1936	rBV	1157605	1699057	68.71%	8.086%
28	14.675	1958	1970	1982	rBV	77689	206925	8.37%	0.985%
29	15.422	2089	2097	2104	rBV	715670	1079912	43.67%	5.139%
30	15.475	2104	2106	2112	rVV7	4591	7616	0.31%	0.036%
31	15.557	2115	2120	2135	rVV	122973	202994	8.21%	0.966%
32	15.663	2135	2138	2142	rVB6	3688	5820	0.24%	0.028%
33	16.204	2226	2230	2234	rVB7	2789	4528	0.18%	0.022%
34	16.645	2302	2305	2310	rVB7	2099	2879	0.12%	0.014%
35	16.728	2317	2319	2328	rVB7	2367	4028	0.16%	0.019%
36	16.969	2356	2360	2364	rVB5	3597	7150	0.29%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019338.D
 Acq On : 12 Jan 2024 19:48
 Operator : MA/JU
 Sample : P1091-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	17.181	2389	2396	2406	rBV	1567102	2176332	88.01%	10.357%
38	17.281	2406	2413	2427	rBV2	799450	1213697	49.08%	5.776%
39	17.575	2461	2463	2465	rBV2	3305	2574	0.10%	0.012%
40	18.075	2544	2548	2554	rBV3	18858	28935	1.17%	0.138%
41	18.316	2587	2589	2590	rBV	3274	2478	0.10%	0.012%
42	19.098	2719	2722	2727	rVB4	12244	16839	0.68%	0.080%
43	19.175	2732	2735	2738	rBV2	10219	14369	0.58%	0.068%
44	19.316	2756	2759	2762	rBV4	14249	19805	0.80%	0.094%
45	19.451	2779	2782	2788	rBV7	10354	17661	0.71%	0.084%
46	19.528	2789	2795	2801	rBV	1142378	1525160	61.67%	7.258%
47	21.286	3089	3094	3100	rBV	1961661	2472908	100.00%	11.769%
48	23.486	3461	3468	3482	rVB2	730630	1511472	61.12%	7.193%
49	23.639	3487	3494	3504	rVB	1228042	2416889	97.73%	11.502%




Sum of corrected areas: 21012529

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019338.D
Acq On : 12 Jan 2024 19:48
Operator : MA/JU
Sample : P1091-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

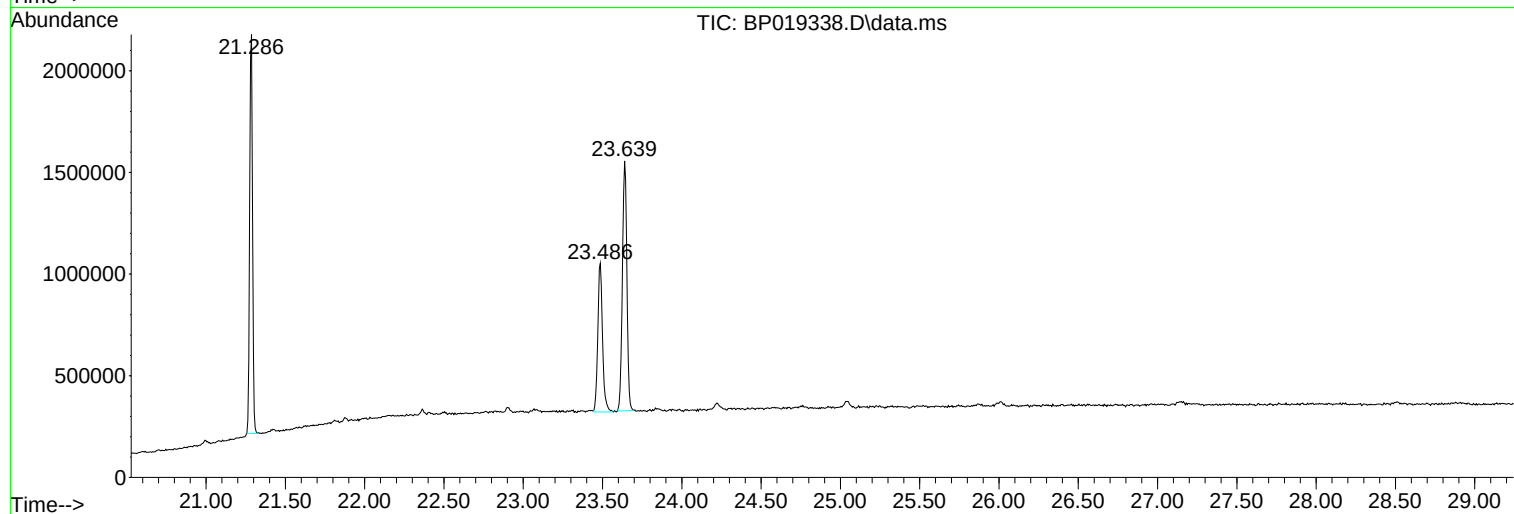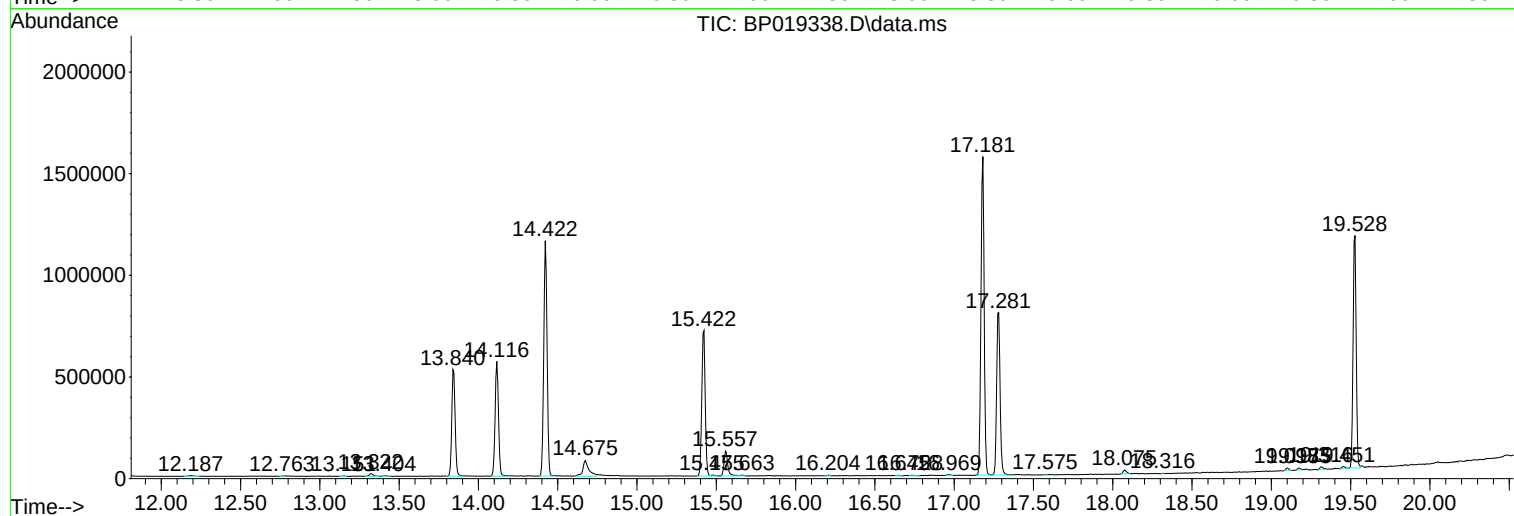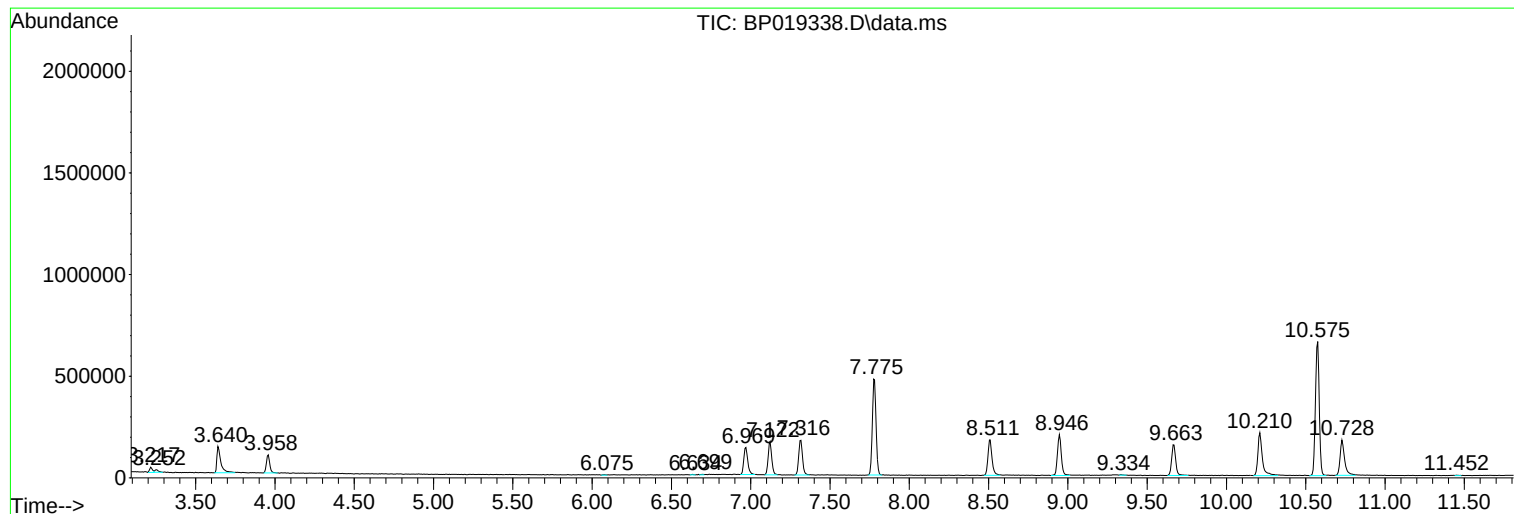

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019338.D
Acq On : 12 Jan 2024 19:48
Operator : MA/JU
Sample : P1091-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.958	3.36 ng/ul	129201	1,4-Dichlorobenzene-d4	7.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Toluene			92	C7H8	000108-88-3	93
2	Toluene			92	C7H8	000108-88-3	93
3	Toluene			92	C7H8	000108-88-3	90
4	Toluene			92	C7H8	000108-88-3	90
5	Toluene			92	C7H8	000108-88-3	87

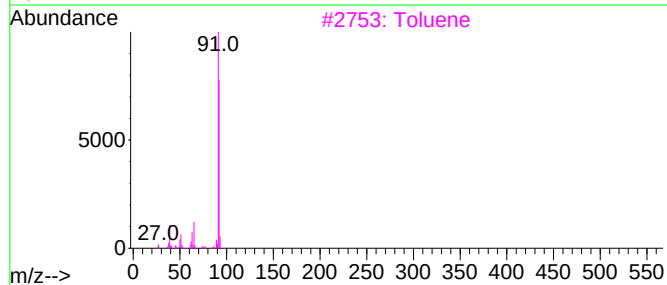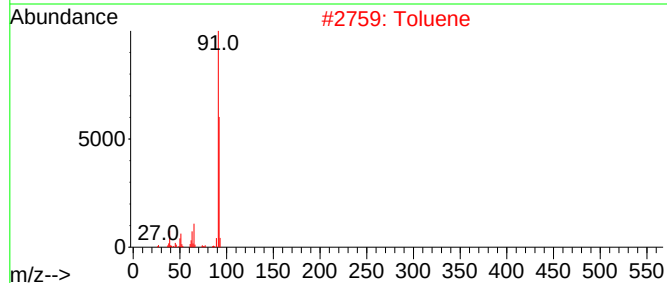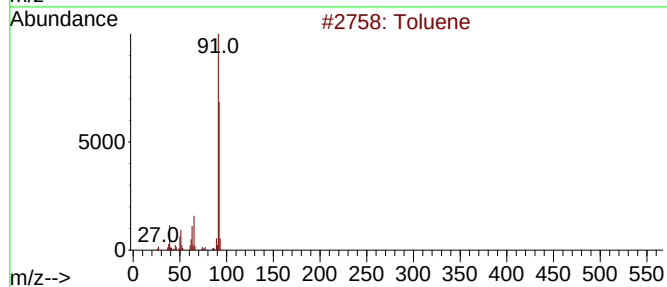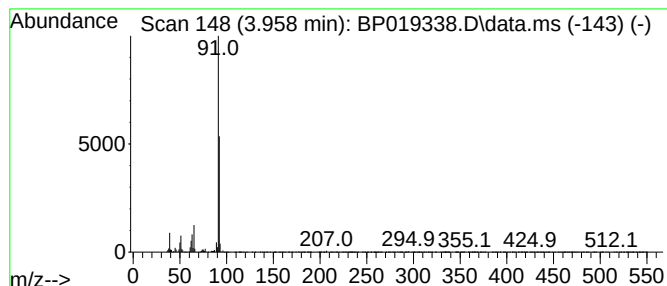

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019338.D
Acq On : 12 Jan 2024 19:48
Operator : MA/JU
Sample : P1091-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	3.958	3.4	ng/ul	129201	1	7.775	767971	20.0