

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019341.D
 Acq On : 12 Jan 2024 21:30
 Operator : MA/JU
 Sample : P1091-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	29	rVB	23265	32412	0.58%	0.080%
2	3.640	91	94	107	rBV	124211	214284	3.86%	0.531%
3	3.858	129	131	138	rVB5	7553	10623	0.19%	0.026%
4	3.952	144	147	153	rBV2	10440	13811	0.25%	0.034%
5	6.822	630	635	639	rBV7	3382	5810	0.10%	0.014%
6	6.970	654	660	670	rVB	115658	191643	3.45%	0.475%
7	7.122	679	686	694	rBV	440381	695274	12.52%	1.723%
8	7.311	712	718	734	rVB	423149	690517	12.43%	1.711%
9	7.417	734	736	741	rBV4	4474	6557	0.12%	0.016%
10	7.775	791	797	807	rBV	420976	690185	12.43%	1.710%
11	8.505	914	921	936	rBV	354830	580376	10.45%	1.438%
12	8.946	988	996	1007	rBV	575477	941500	16.95%	2.333%
13	9.293	1051	1055	1059	rBV7	5840	10822	0.19%	0.027%
14	9.340	1061	1063	1071	rVB7	3996	7013	0.13%	0.017%
15	9.663	1112	1118	1128	rBV	478862	782986	14.10%	1.940%
16	10.205	1202	1210	1228	rBV	647469	1151050	20.72%	2.852%
17	10.569	1264	1272	1285	rVB	595294	1007560	18.14%	2.497%
18	10.722	1290	1298	1316	rBV	554597	1029926	18.54%	2.552%
19	12.175	1538	1545	1551	rBV2	10191	22171	0.40%	0.055%
20	12.775	1643	1647	1652	rVB8	3021	5606	0.10%	0.014%
21	13.322	1735	1740	1746	rVB2	13162	21986	0.40%	0.054%
22	13.840	1820	1828	1839	rBV	1389803	2018872	36.35%	5.003%
23	14.116	1867	1875	1886	rBV	1526628	2157307	38.84%	5.346%
24	14.422	1920	1927	1940	rBV	999304	1459041	26.27%	3.616%
25	14.669	1963	1969	1986	rBV	101025	227575	4.10%	0.564%
26	14.875	2000	2004	2011	rVB9	5094	10412	0.19%	0.026%
27	15.416	2089	2096	2105	rBV	2089344	3015997	54.30%	7.474%
28	15.557	2114	2120	2133	rBV	950789	1308347	23.56%	3.242%
29	15.657	2133	2137	2144	rVB6	11258	18774	0.34%	0.047%
30	15.934	2179	2184	2189	rBV8	6467	9880	0.18%	0.024%
31	16.198	2226	2229	2238	rVB6	7580	11841	0.21%	0.029%
32	16.598	2294	2297	2301	rBV5	3032	6010	0.11%	0.015%
33	16.722	2314	2318	2322	rBV6	6937	9738	0.18%	0.024%
34	16.775	2322	2327	2333	rVV	28775	40418	0.73%	0.100%
35	16.851	2337	2340	2347	rVB8	6152	9641	0.17%	0.024%
36	16.969	2357	2360	2367	rBV8	3940	7065	0.13%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019341.D
Acq On : 12 Jan 2024 21:30
Operator : MA/JU
Sample : P1091-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B45

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	17.181	2387	2396	2403	rBV	1372949	1986622	35.77%	4.923%
38	17.281	2406	2413	2425	rVV	2927910	4059199	73.08%	10.059%
39	17.575	2461	2463	2469	rVB7	3907	6553	0.12%	0.016%
40	17.851	2507	2510	2514	rBV5	7189	8144	0.15%	0.020%
41	18.075	2543	2548	2555	rBV3	34182	50757	0.91%	0.126%
42	19.098	2718	2722	2728	rBV2	44805	68082	1.23%	0.169%
43	19.169	2731	2734	2741	rVV	39005	55787	1.00%	0.138%
44	19.310	2755	2758	2761	rBV4	27678	33045	0.59%	0.082%
45	19.528	2789	2795	2801	rBV	4272391	5362333	96.54%	13.288%
46	21.281	3088	3093	3100	rBV	1855105	2416720	43.51%	5.989%
47	23.486	3461	3468	3478	rVB	2914784	5554315	100.00%	13.764%
48	23.639	3487	3494	3502	rVB	1162233	2329551	41.94%	5.773%




Sum of corrected areas: 40354138

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019341.D
Acq On : 12 Jan 2024 21:30
Operator : MA/JU
Sample : P1091-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

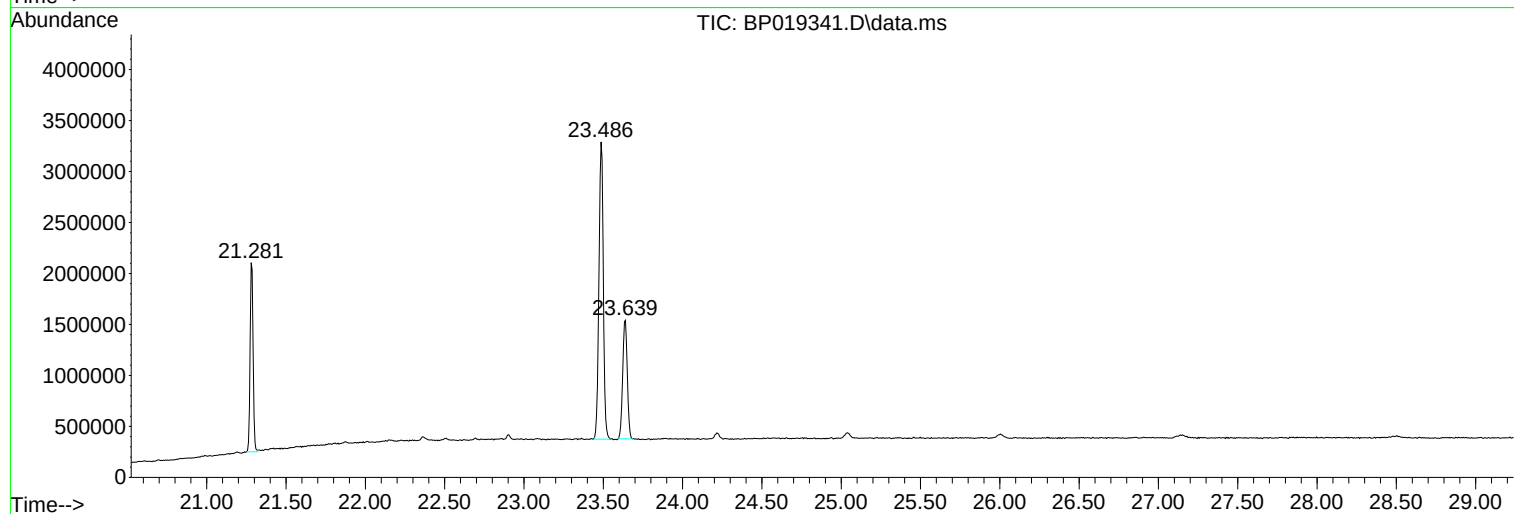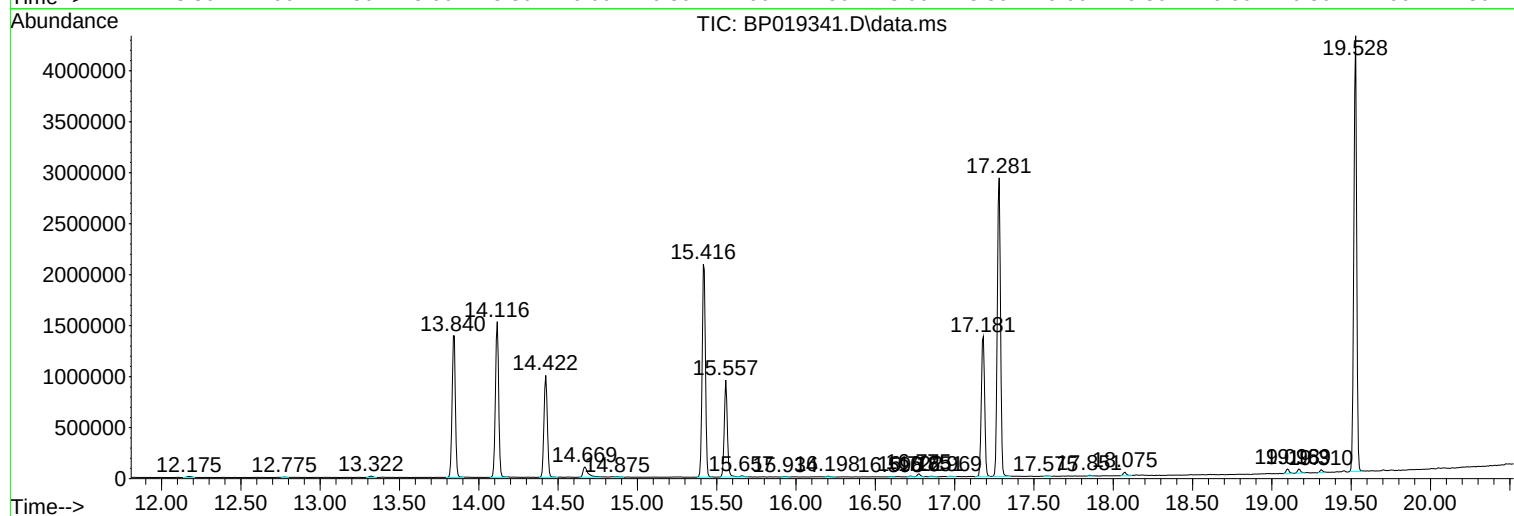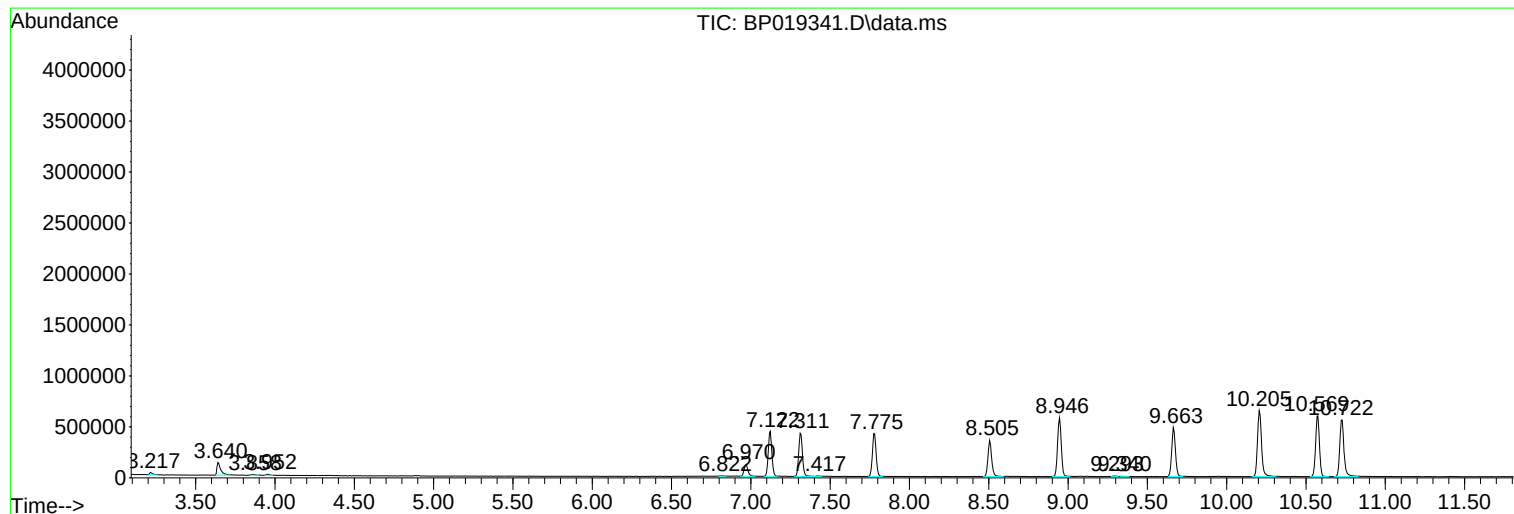

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019341.D
Acq On : 12 Jan 2024 21:30
Operator : MA/JU
Sample : P1091-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019341.D
Acq On : 12 Jan 2024 21:30
Operator : MA/JU
Sample : P1091-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc