

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019344.D
 Acq On : 12 Jan 2024 23:13
 Operator : MA/JU
 Sample : P1091-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	32	rVB	20227	29721	0.66%	0.083%
2	3.640	91	94	106	rBV	91091	155540	3.48%	0.436%
3	3.958	145	148	152	rVB2	7449	9593	0.21%	0.027%
4	6.816	629	634	641	rBV6	6967	13358	0.30%	0.037%
5	6.969	653	660	670	rBV	107639	179082	4.01%	0.502%
6	7.122	679	686	700	rBV	408770	638213	14.27%	1.789%
7	7.310	710	718	727	rBV	385366	618304	13.83%	1.733%
8	7.405	730	734	739	rVV2	17914	31308	0.70%	0.088%
9	7.775	789	797	806	rBV	392117	632426	14.14%	1.773%
10	8.504	911	921	934	rBV	320122	545214	12.19%	1.529%
11	8.946	988	996	1006	rBV	528168	868852	19.43%	2.436%
12	9.075	1014	1018	1025	rBV4	9161	15270	0.34%	0.043%
13	9.293	1051	1055	1061	rBV8	4882	8115	0.18%	0.023%
14	9.663	1111	1118	1128	rBV	446081	726972	16.26%	2.038%
15	9.940	1157	1165	1171	rBV	3900	11013	0.25%	0.031%
16	10.204	1202	1210	1224	rBV	608467	1064952	23.82%	2.986%
17	10.575	1262	1273	1283	rBV	546942	907760	20.30%	2.545%
18	10.728	1291	1299	1312	rBV	486948	904567	20.23%	2.536%
19	11.410	1408	1415	1416	rBV7	3942	6103	0.14%	0.017%
20	12.175	1539	1545	1556	rVB4	10382	20475	0.46%	0.057%
21	12.781	1643	1648	1653	rVB9	3976	7170	0.16%	0.020%
22	13.028	1685	1690	1695	rVB9	3255	5724	0.13%	0.016%
23	13.322	1734	1740	1746	rVB3	14846	23817	0.53%	0.067%
24	13.398	1746	1753	1756	rBV7	3598	8151	0.18%	0.023%
25	13.845	1822	1829	1840	rBV	1380773	1951754	43.65%	5.472%
26	14.116	1864	1875	1884	rBV	1484624	2096665	46.89%	5.878%
27	14.422	1920	1927	1933	rBV	913485	1300942	29.10%	3.647%
28	14.669	1963	1969	1986	rBV2	84602	193830	4.34%	0.543%
29	14.851	1993	2000	2006	rVB2	4478	9879	0.22%	0.028%
30	15.222	2059	2063	2066	rBV5	3804	5502	0.12%	0.015%
31	15.251	2066	2068	2075	rVB4	5387	9646	0.22%	0.027%
32	15.422	2089	2097	2111	rBV	2019869	2876833	64.34%	8.065%
33	15.557	2113	2120	2134	rBV	795718	1114674	24.93%	3.125%
34	15.663	2134	2138	2144	rVB2	8789	14160	0.32%	0.040%
35	15.933	2179	2184	2190	rBV6	15905	25170	0.56%	0.071%
36	16.145	2217	2220	2225	rVV7	2724	4552	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019344.D
 Acq On : 12 Jan 2024 23:13
 Operator : MA/JU
 Sample : P1091-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	16.204	2226	2230	2236	rVB6	8744	12051	0.27%	0.034%
38	16.775	2322	2327	2334	rVB2	45416	62683	1.40%	0.176%
39	16.857	2334	2341	2344	rBV9	5270	8838	0.20%	0.025%
40	17.104	2380	2383	2388	rVB7	4457	7085	0.16%	0.020%
41	17.180	2388	2396	2405	rBV	1257804	1757203	39.30%	4.926%
42	17.280	2406	2413	2423	rBV	2482974	3515210	78.62%	9.855%
43	17.475	2443	2446	2450	rVB6	5291	6764	0.15%	0.019%
44	18.075	2542	2548	2555	rBV2	65790	106002	2.37%	0.297%
45	18.145	2557	2560	2563	rVB	8072	11905	0.27%	0.033%
46	18.351	2590	2595	2597	rBV6	8055	11051	0.25%	0.031%
47	18.398	2601	2603	2607	rVB4	5383	7128	0.16%	0.020%
48	19.098	2718	2722	2729	rBV3	38195	50387	1.13%	0.141%
49	19.174	2731	2735	2741	rBV	37645	61979	1.39%	0.174%
50	19.316	2755	2759	2764	rBV2	54028	76734	1.72%	0.215%
51	19.527	2789	2795	2801	rBV	3378918	4471260	100.00%	12.535%
52	21.286	3089	3094	3101	rBV	1616844	2039051	45.60%	5.717%
53	23.486	3461	3468	3479	rVB2	2265315	4422131	98.90%	12.398%
54	23.639	3487	3494	3506	rVB	996196	2006568	44.88%	5.625%




Sum of corrected areas: 35669337

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019344.D
Acq On : 12 Jan 2024 23:13
Operator : MA/JU
Sample : P1091-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

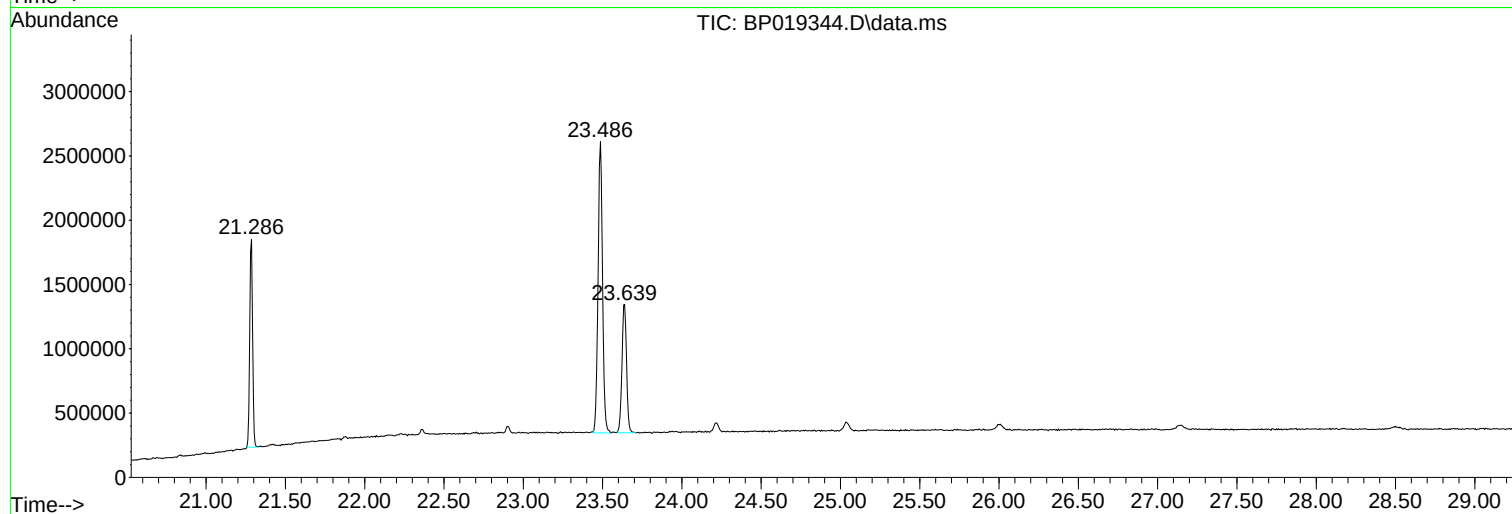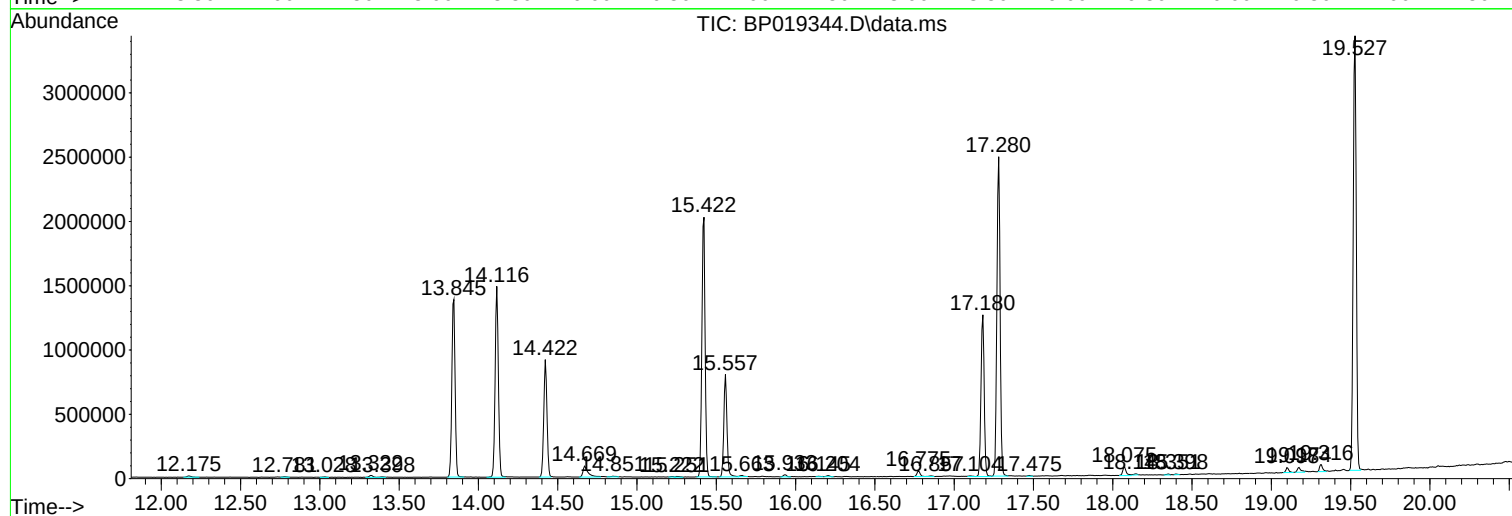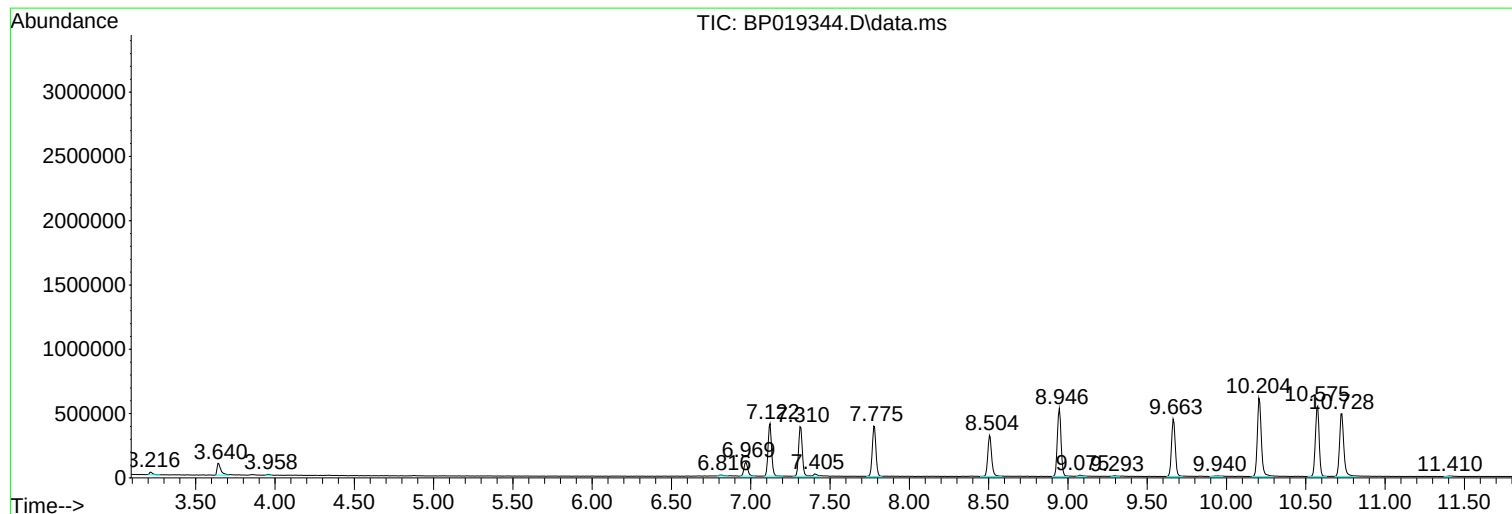

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019344.D
Acq On : 12 Jan 2024 23:13
Operator : MA/JU
Sample : P1091-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019344.D
Acq On : 12 Jan 2024 23:13
Operator : MA/JU
Sample : P1091-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc