

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019345.D
 Acq On : 12 Jan 2024 23:47
 Operator : MA/JU
 Sample : P1091-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	30	rVB	28120	37367	0.83%	0.100%
2	3.640	90	94	104	rBV	162165	252626	5.59%	0.677%
3	3.858	127	131	135	rBV3	8034	12184	0.27%	0.033%
4	3.958	144	148	155	rVB2	8928	13687	0.30%	0.037%
5	4.905	307	309	313	rVB5	5074	6687	0.15%	0.018%
6	6.811	630	633	638	rBV5	3794	6950	0.15%	0.019%
7	6.969	654	660	673	rVB	142767	242446	5.36%	0.650%
8	7.116	678	685	698	rVB	507333	812555	17.98%	2.177%
9	7.311	711	718	731	rBV	499969	811181	17.95%	2.173%
10	7.422	733	737	741	rVB5	3843	6390	0.14%	0.017%
11	7.775	791	797	807	rBV	381928	613912	13.58%	1.645%
12	8.505	914	921	934	rBV	421827	690696	15.28%	1.851%
13	8.946	988	996	1008	rBV	666310	1091354	24.15%	2.924%
14	9.293	1049	1055	1061	rBV9	5153	10557	0.23%	0.028%
15	9.663	1111	1118	1128	rBV	572993	917625	20.31%	2.459%
16	10.205	1201	1210	1223	rBV	768983	1318473	29.18%	3.532%
17	10.569	1260	1272	1282	rBV	505428	867533	19.20%	2.324%
18	10.722	1291	1298	1313	rBV	660460	1189684	26.33%	3.187%
19	11.416	1408	1416	1417	rBV7	3857	7201	0.16%	0.019%
20	12.169	1540	1544	1553	rVB2	11693	21882	0.48%	0.059%
21	13.322	1733	1740	1747	rBV	17295	28879	0.64%	0.077%
22	13.393	1748	1752	1758	rBV8	3589	6850	0.15%	0.018%
23	13.845	1820	1829	1838	rBV	1540910	2172119	48.06%	5.820%
24	14.116	1867	1875	1887	rBV	1649310	2408474	53.29%	6.453%
25	14.422	1921	1927	1934	rBV	848014	1205910	26.68%	3.231%
26	14.563	1947	1951	1955	rVB6	2626	4829	0.11%	0.013%
27	14.669	1962	1969	1987	rBV2	92471	221628	4.90%	0.594%
28	15.422	2090	2097	2104	rBV	2237231	3177551	70.31%	8.513%
29	15.557	2112	2120	2134	rBV	829197	1140612	25.24%	3.056%
30	15.663	2134	2138	2143	rVB2	10682	17407	0.39%	0.047%
31	15.928	2178	2183	2188	rBV7	10809	19436	0.43%	0.052%
32	15.987	2188	2193	2197	rVB7	3042	6452	0.14%	0.017%
33	16.204	2226	2230	2234	rVB5	8662	12032	0.27%	0.032%
34	16.775	2321	2327	2332	rBV	39782	57020	1.26%	0.153%
35	16.851	2336	2340	2345	rBV7	7585	12277	0.27%	0.033%
36	16.910	2345	2350	2356	rBV	122229	161847	3.58%	0.434%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019345.D
 Acq On : 12 Jan 2024 23:47
 Operator : MA/JU
 Sample : P1091-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	17.181	2389	2396	2406	rBV	1193550	1606185	35.54%	4.303%
38	17.281	2406	2413	2425	rBV	2617713	3608428	79.85%	9.668%
39	17.851	2507	2510	2513	rBV5	3398	4759	0.11%	0.013%
40	17.951	2523	2527	2530	rBV6	3147	5218	0.12%	0.014%
41	18.075	2542	2548	2555	rBV	49195	82934	1.84%	0.222%
42	18.139	2557	2559	2564	rVB4	4983	7230	0.16%	0.019%
43	19.098	2718	2722	2727	rBV3	37909	51018	1.13%	0.137%
44	19.175	2730	2735	2741	rBV2	37870	66513	1.47%	0.178%
45	19.310	2754	2758	2765	rBV4	58571	85598	1.89%	0.229%
46	19.451	2780	2782	2787	rVB6	11633	11782	0.26%	0.032%
47	19.528	2789	2795	2807	rVV	3409529	4519145	100.00%	12.108%
48	21.286	3089	3094	3101	rVB	1397996	1788839	39.58%	4.793%
49	23.486	3461	3468	3481	rVB	2184519	4192334	92.77%	11.232%
50	23.639	3487	3494	3506	rVB	860308	1710212	37.84%	4.582%




Sum of corrected areas: 37324508

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019345.D
Acq On : 12 Jan 2024 23:47
Operator : MA/JU
Sample : P1091-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

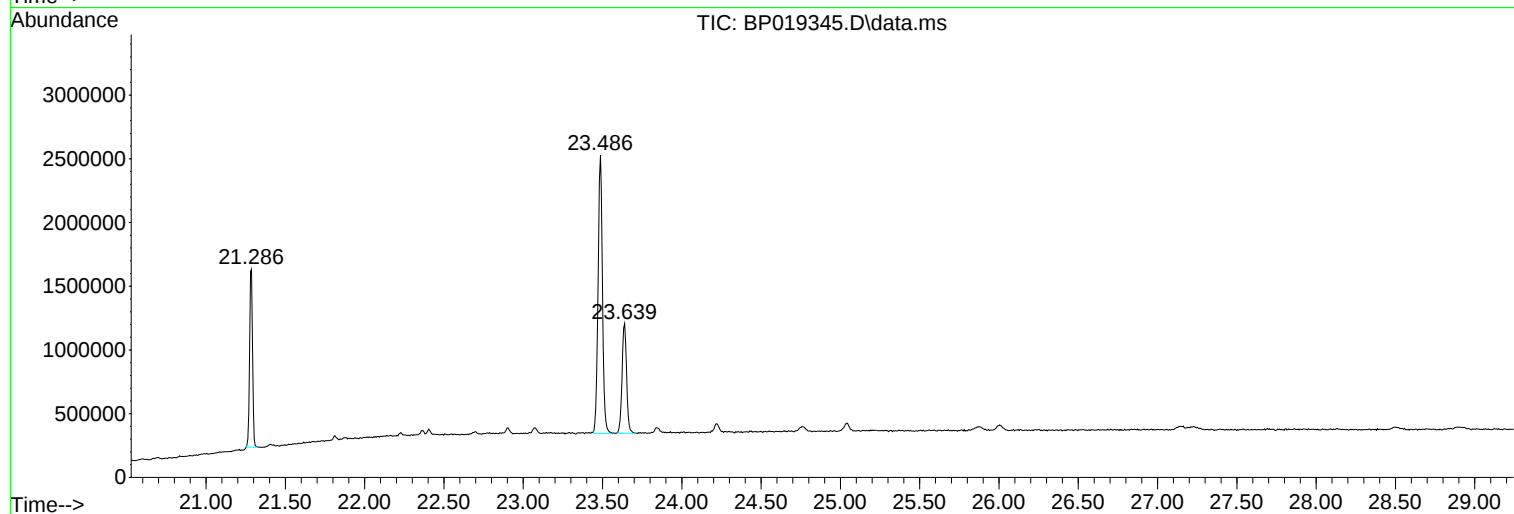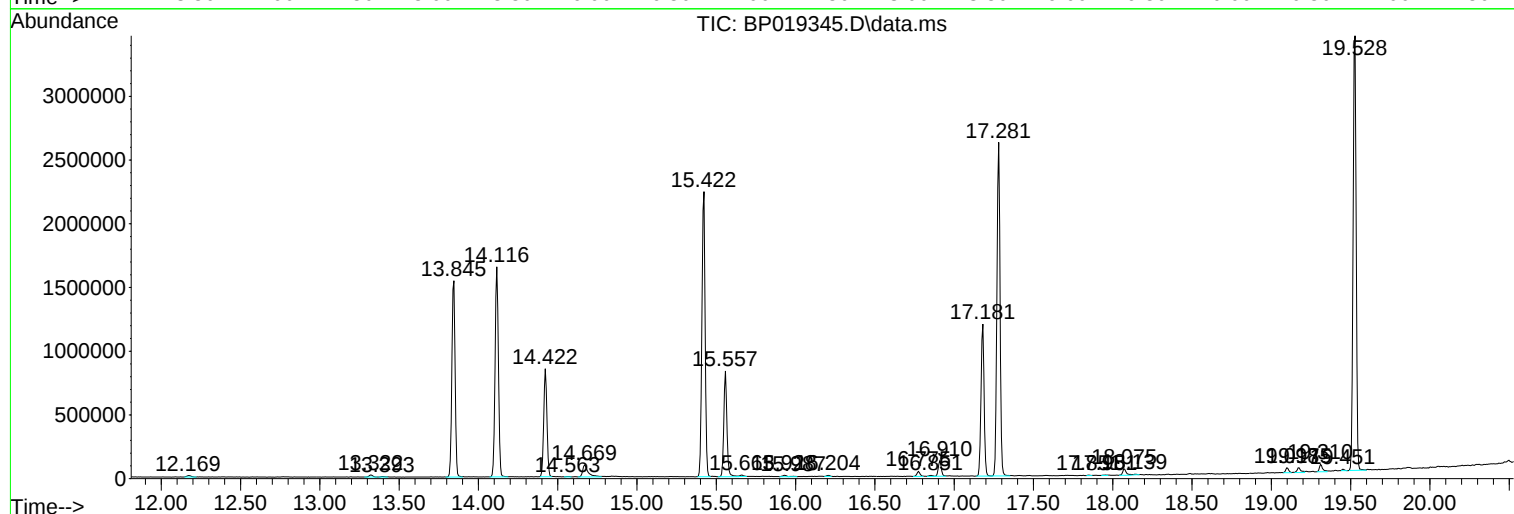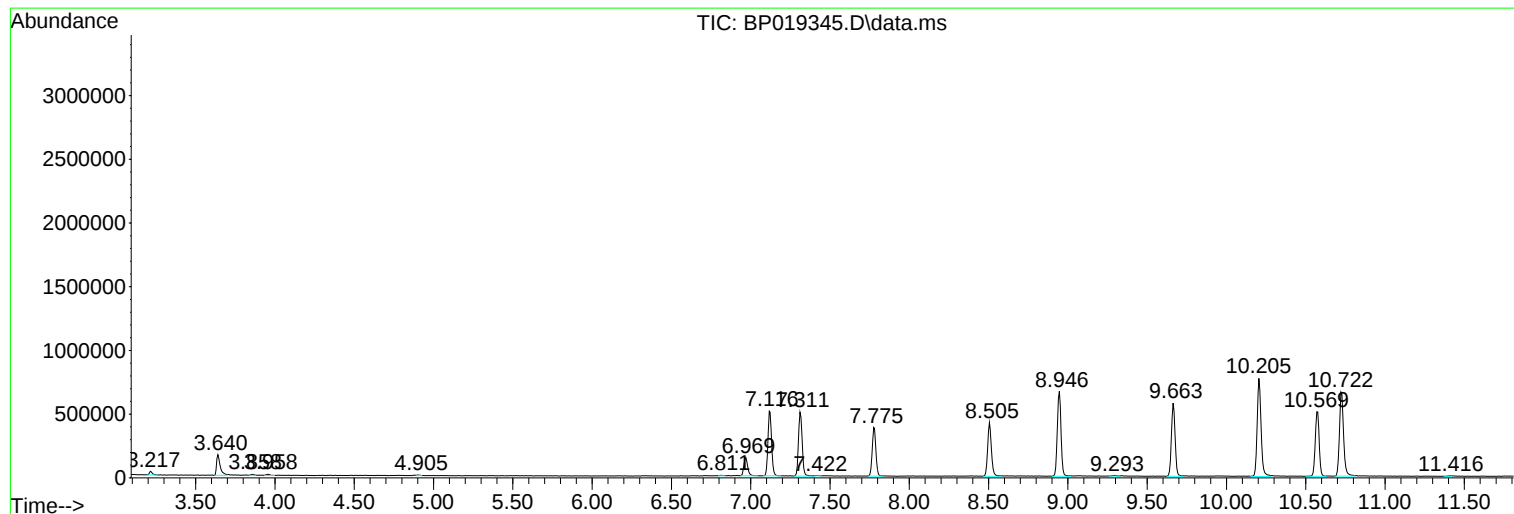

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019345.D
Acq On : 12 Jan 2024 23:47
Operator : MA/JU
Sample : P1091-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzyl Benzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.910	2.02 ng/ul	161847	Phenanthrene-d10	17.181

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzyl Benzoate	212	C14H12O2	000120-51-4	95
2			Benzyl Benzoate	212	C14H12O2	000120-51-4	93
3			Benzyl Benzoate	212	C14H12O2	000120-51-4	90
4			Benzoic acid, 2-phenylhydrazide	212	C13H12N2O	000532-96-7	64
5			Benzyl Benzoate	212	C14H12O2	000120-51-4	64

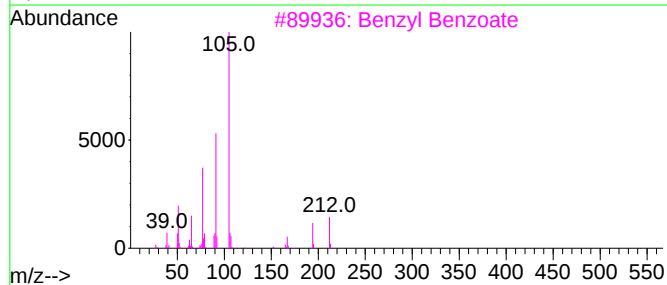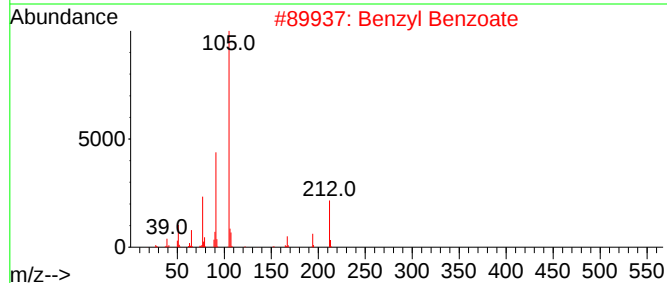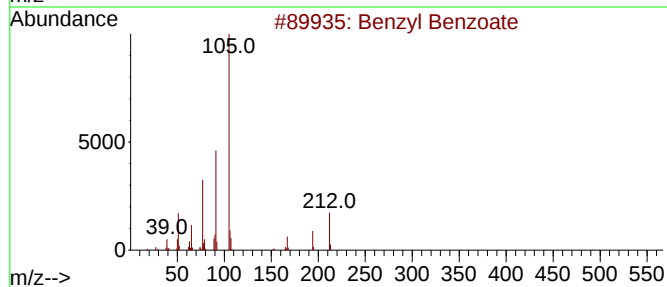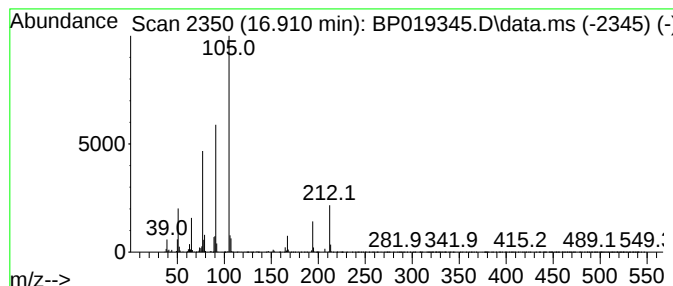

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019345.D
Acq On : 12 Jan 2024 23:47
Operator : MA/JU
Sample : P1091-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzyl Benzoate	16.910	2.0	ng/ul	161847	4	17.181	1606190	20.0