

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019352.D
 Acq On : 13 Jan 2024 04:19
 Operator : MA/JU
 Sample : PB158383BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK383

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	30	rVB	30997	43480	1.05%	0.113%
2	3.634	90	93	114	rBV	448556	728792	17.58%	1.900%
3	3.952	144	147	153	rVB2	8540	11892	0.29%	0.031%
4	6.834	633	637	640	rBV5	3002	5782	0.14%	0.015%
5	6.964	652	659	670	rBV	566641	899118	21.69%	2.344%
6	7.116	677	685	698	rVB	438187	687024	16.57%	1.791%
7	7.311	712	718	729	rBV	538142	857282	20.68%	2.235%
8	7.775	789	797	806	rBV	394400	627024	15.12%	1.635%
9	8.505	914	921	932	rBV	692148	1124920	27.13%	2.933%
10	8.946	988	996	1007	rBV	556526	929280	22.41%	2.423%
11	9.663	1109	1118	1130	rBV	502145	825761	19.92%	2.153%
12	10.205	1200	1210	1229	rBV	722150	1246235	30.06%	3.249%
13	10.569	1264	1272	1283	rBV	541667	905858	21.85%	2.362%
14	10.722	1290	1298	1312	rBV	669573	1207525	29.13%	3.148%
15	11.834	1484	1487	1494	rVB8	2898	5279	0.13%	0.014%
16	12.175	1538	1545	1554	rBV3	9999	21111	0.51%	0.055%
17	13.316	1735	1739	1745	rBV4	8621	14240	0.34%	0.037%
18	13.840	1820	1828	1840	rBV	1474023	2086780	50.33%	5.441%
19	14.116	1867	1875	1887	rBV	1516222	2269783	54.75%	5.918%
20	14.422	1920	1927	1936	rBV	1006957	1400834	33.79%	3.652%
21	14.557	1945	1950	1953	rBV5	2676	4237	0.10%	0.011%
22	14.657	1960	1967	1995	rBV	597004	1036127	24.99%	2.702%
23	15.416	2086	2096	2107	rBV	2043238	2991981	72.17%	7.801%
24	15.557	2113	2120	2132	rBV	737049	1030460	24.86%	2.687%
25	15.657	2132	2137	2147	rVB3	11394	25416	0.61%	0.066%
26	16.204	2226	2230	2238	rVB5	8495	12448	0.30%	0.032%
27	16.851	2336	2340	2347	rBV10	4636	7123	0.17%	0.019%
28	16.969	2354	2360	2362	rBV6	4807	7694	0.19%	0.020%
29	17.181	2388	2396	2405	rBV	1243745	1801133	43.44%	4.696%
30	17.281	2405	2413	2422	rBV	2254999	3254603	78.50%	8.486%
31	18.075	2546	2548	2553	rBV6	5556	7004	0.17%	0.018%
32	19.098	2718	2722	2728	rVB2	32988	44738	1.08%	0.117%
33	19.169	2731	2734	2739	rVV	26192	34728	0.84%	0.091%
34	19.310	2756	2758	2761	rBV4	7799	8743	0.21%	0.023%
35	19.528	2788	2795	2804	rBV	3118790	4145796	100.00%	10.809%
36	21.286	3089	3094	3101	rVB	1613285	2066972	49.86%	5.389%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019352.D
Acq On : 13 Jan 2024 04:19
Operator : MA/JU
Sample : PB158383BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK383

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	23.486	3461	3468	3481	rVB	2067294	4003340	96.56%	10.438%
38	23.639	3488	3494	3504	rVB	1037299	1972994	47.59%	5.144%




Sum of corrected areas: 38353537

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019352.D
Acq On : 13 Jan 2024 04:19
Operator : MA/JU
Sample : PB158383BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

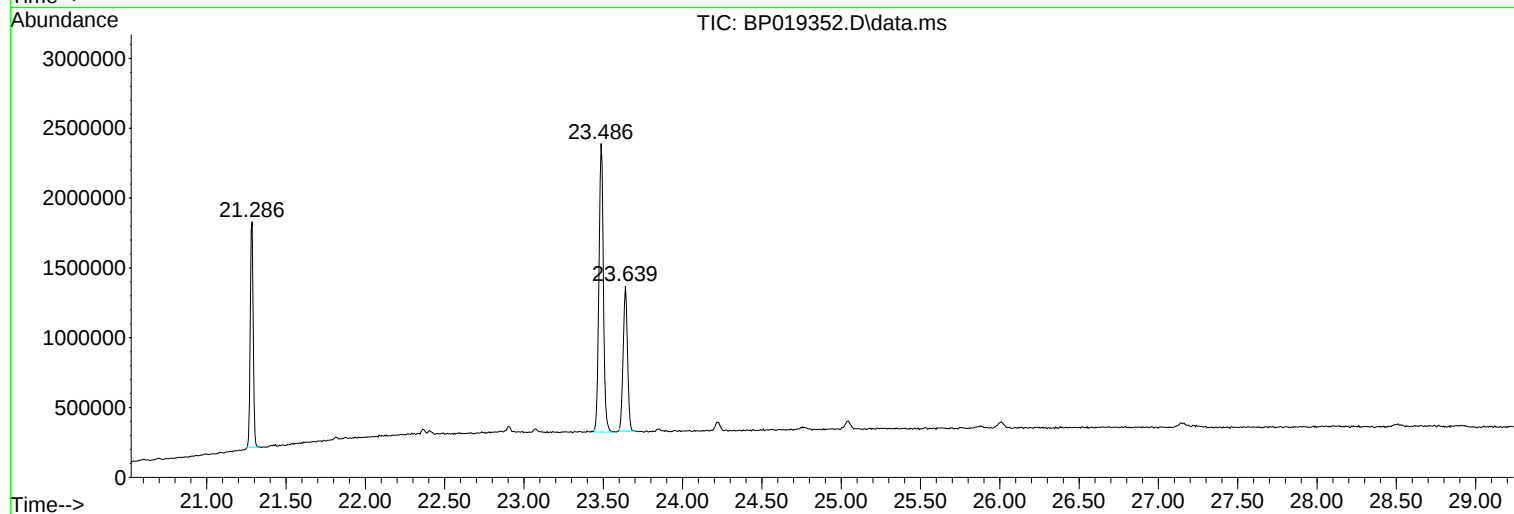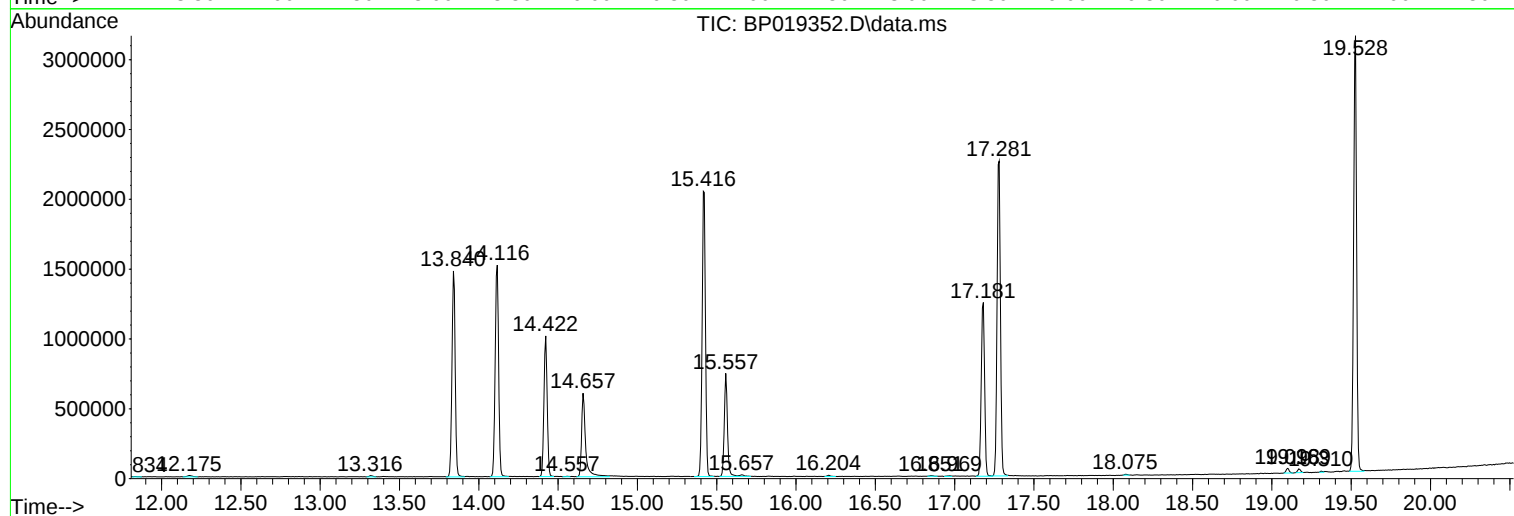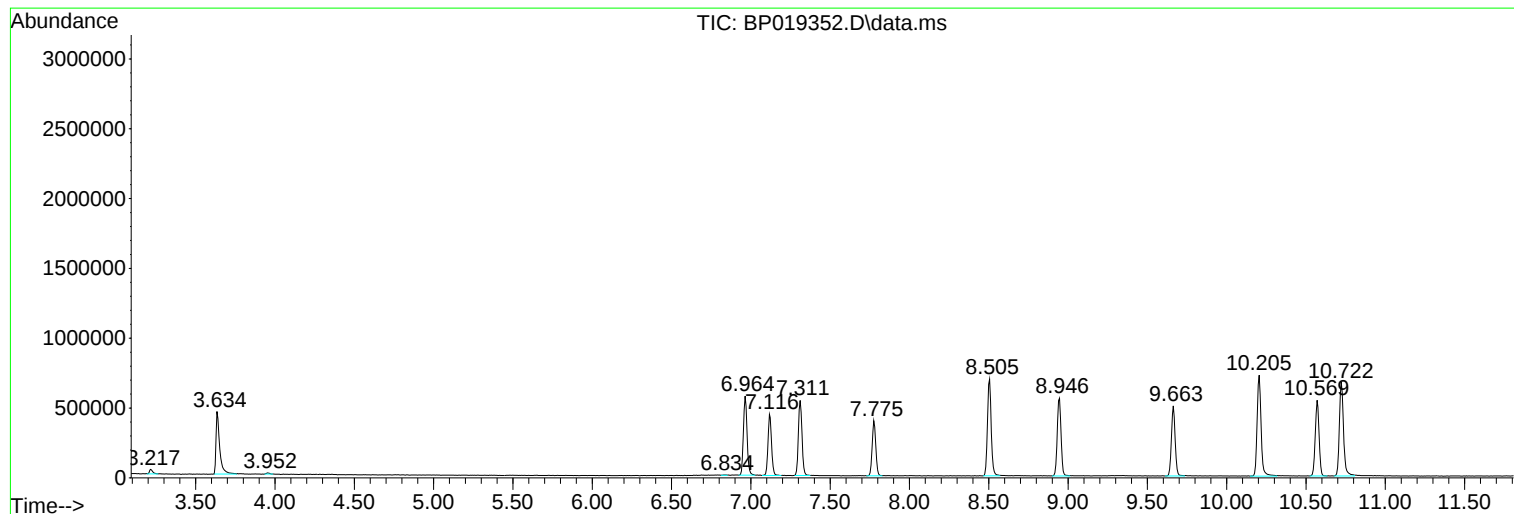

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019352.D
Acq On : 13 Jan 2024 04:19
Operator : MA/JU
Sample : PB158383BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019352.D
Acq On : 13 Jan 2024 04:19
Operator : MA/JU
Sample : PB158383BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------