

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019355.D
 Acq On : 13 Jan 2024 06:01
 Operator : MA/JU
 Sample : P1091-18
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	28	rVB	26377	34702	0.60%	0.076%
2	3.640	90	94	110	rBV	163347	282740	4.89%	0.616%
3	3.952	144	147	151	rBV3	7071	8811	0.15%	0.019%
4	6.963	654	659	669	rVB	128647	211468	3.66%	0.461%
5	7.116	678	685	698	rVB	567558	881118	15.25%	1.920%
6	7.310	711	718	730	rBV	532143	840070	14.54%	1.830%
7	7.775	787	797	805	rBV	468978	733772	12.70%	1.599%
8	8.505	914	921	937	rBV	399686	659041	11.41%	1.436%
9	8.940	989	995	1010	rBV	729346	1211429	20.97%	2.639%
10	9.334	1060	1062	1070	rVB6	3972	6790	0.12%	0.015%
11	9.663	1109	1118	1135	rBV	635649	1032116	17.87%	2.249%
12	10.204	1202	1210	1233	rBV	828312	1454330	25.17%	3.168%
13	10.569	1264	1272	1286	rBV	631788	1048756	18.15%	2.285%
14	10.722	1290	1298	1317	rBV	717959	1280569	22.17%	2.790%
15	11.422	1409	1417	1419	rBV9	3946	7997	0.14%	0.017%
16	12.175	1539	1545	1550	rBV2	13789	24911	0.43%	0.054%
17	13.051	1690	1694	1702	rVB9	4586	10229	0.18%	0.022%
18	13.316	1734	1739	1746	rVB3	13395	23590	0.41%	0.051%
19	13.392	1746	1752	1755	rBV7	3563	6389	0.11%	0.014%
20	13.840	1820	1828	1840	rBV	1904142	2664966	46.13%	5.806%
21	14.116	1866	1875	1882	rBV	2031764	2977188	51.53%	6.486%
22	14.422	1920	1927	1936	rBV	1116715	1610332	27.87%	3.508%
23	14.663	1962	1968	1980	rBV	92616	203006	3.51%	0.442%
24	14.875	2001	2004	2009	rVB6	4021	6036	0.10%	0.013%
25	15.416	2089	2096	2105	rBV	2750784	3940963	68.22%	8.586%
26	15.557	2113	2120	2132	rBV	993284	1406780	24.35%	3.065%
27	15.657	2134	2137	2144	rVB5	14082	22149	0.38%	0.048%
28	16.204	2225	2230	2238	rBV4	11017	16513	0.29%	0.036%
29	16.722	2312	2318	2322	rBV9	2854	6610	0.11%	0.014%
30	16.851	2332	2340	2346	rBV9	11547	23675	0.41%	0.052%
31	16.933	2350	2354	2357	rBV5	3709	6122	0.11%	0.013%
32	16.963	2357	2359	2366	rVB6	3777	6905	0.12%	0.015%
33	17.181	2389	2396	2403	rBV	1516172	2178659	37.71%	4.746%
34	17.281	2406	2413	2427	rVV	3248494	4567597	79.06%	9.951%
35	17.398	2429	2433	2436	rVB6	7944	11498	0.20%	0.025%
36	17.569	2456	2462	2463	rBV6	8592	10058	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019355.D
Acq On : 13 Jan 2024 06:01
Operator : MA/JU
Sample : P1091-18
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	17.798	2498	2501	2505	rVB5	5446	6843	0.12%	0.015%
38	18.075	2543	2548	2555	rBV5	31166	48733	0.84%	0.106%
39	18.486	2614	2618	2623	rBV4	14620	21426	0.37%	0.047%
40	19.098	2718	2722	2727	rBV	50564	67371	1.17%	0.147%
41	19.175	2730	2735	2738	rBV	43833	66589	1.15%	0.145%
42	19.310	2755	2758	2763	rBV5	23716	34068	0.59%	0.074%
43	19.527	2789	2795	2805	rBV	4477644	5777228	100.00%	12.586%
44	21.286	3089	3094	3101	rBV	2030043	2499570	43.27%	5.445%
45	23.492	3461	3469	3479	rVB	2864502	5556103	96.17%	12.104%
46	23.639	3487	3494	3504	rVB	1246198	2405790	41.64%	5.241%




Sum of corrected areas: 45901606

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019355.D
Acq On : 13 Jan 2024 06:01
Operator : MA/JU
Sample : P1091-18
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

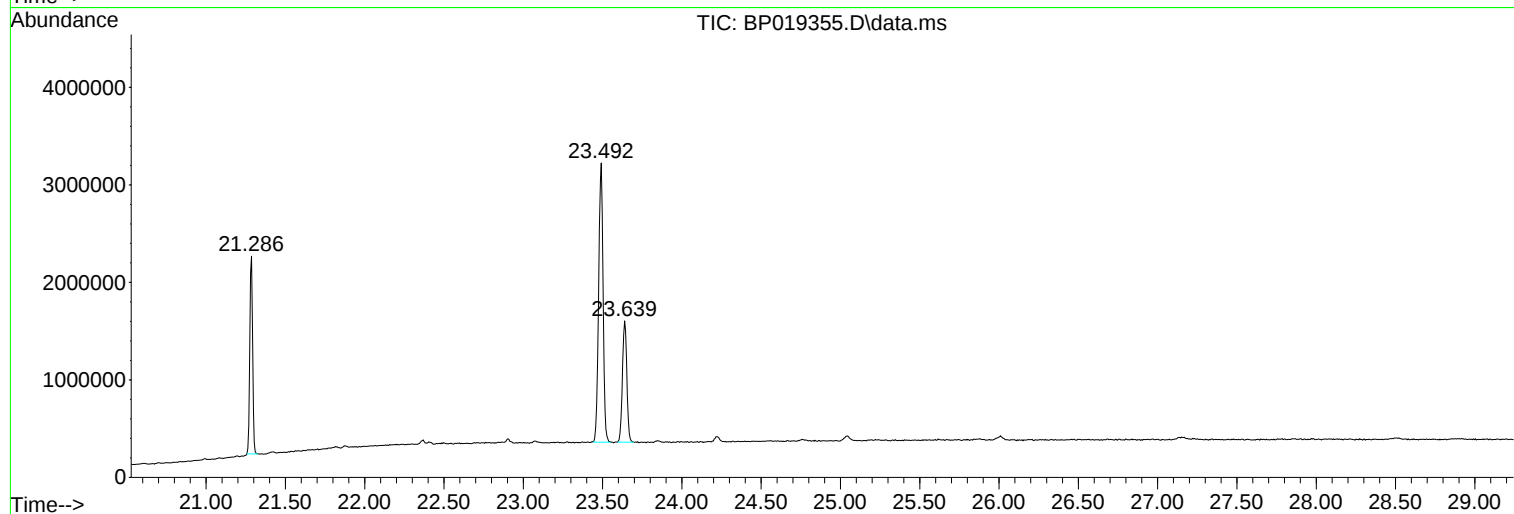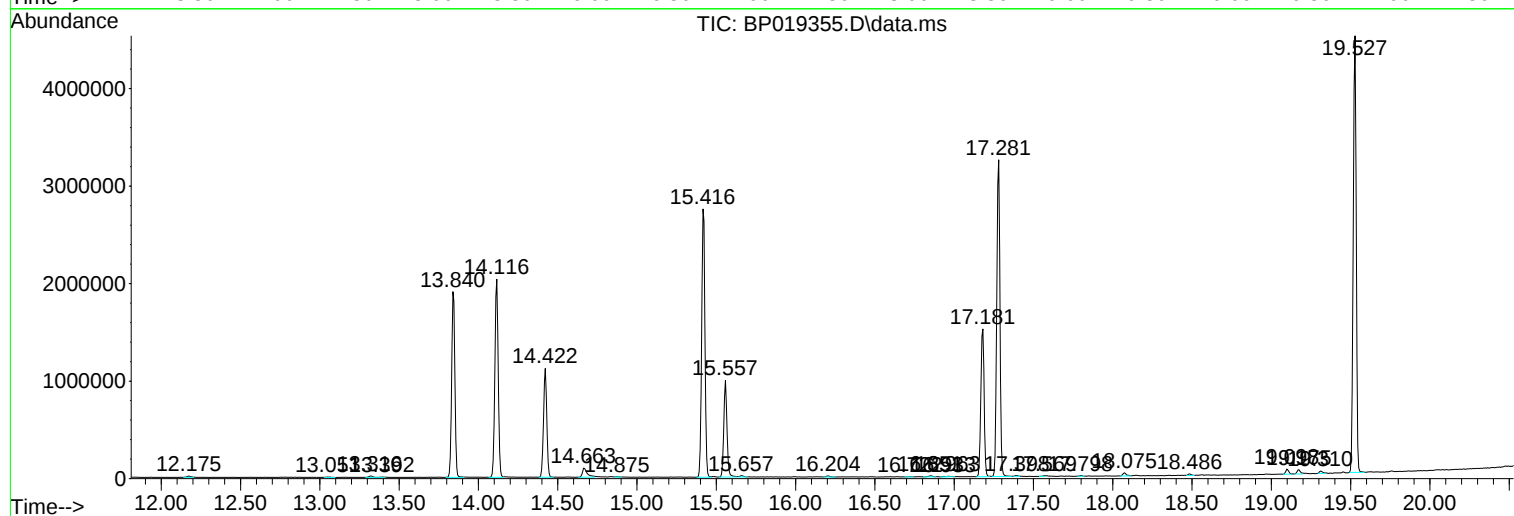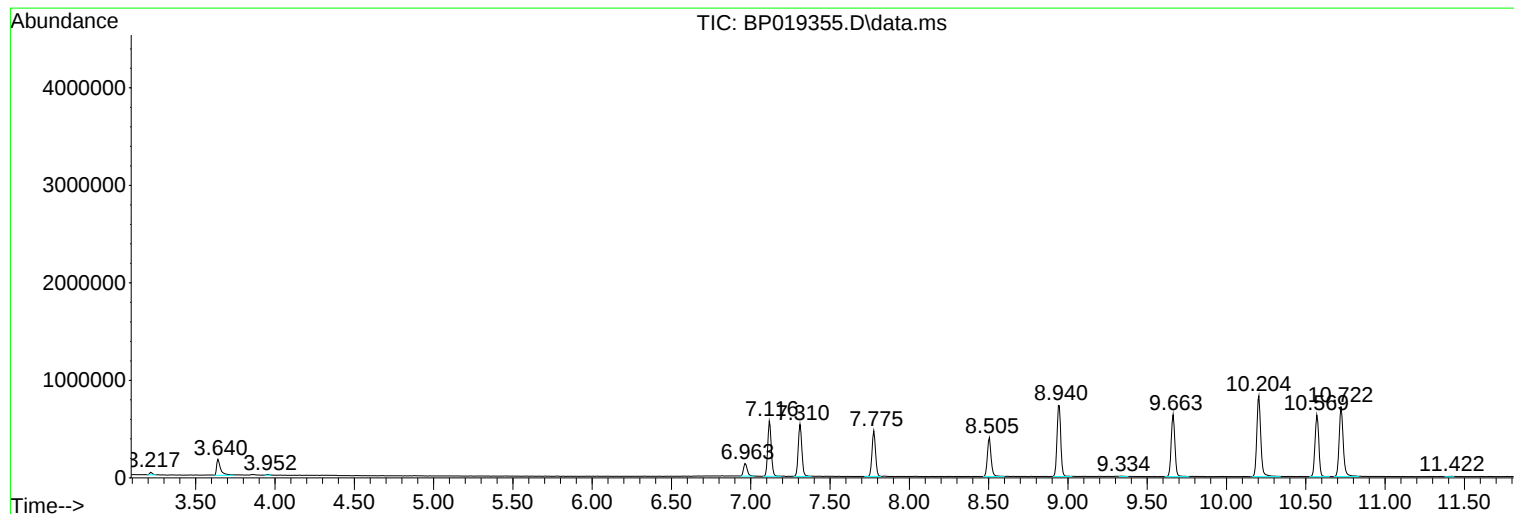

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019355.D
Acq On : 13 Jan 2024 06:01
Operator : MA/JU
Sample : P1091-18
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019355.D
Acq On : 13 Jan 2024 06:01
Operator : MA/JU
Sample : P1091-18
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc