

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019356.D
 Acq On : 13 Jan 2024 06:35
 Operator : MA/JU
 Sample : P1091-19
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	31	rBV	24927	34930	0.63%	0.081%
2	3.646	91	95	112	rBV	74527	148354	2.67%	0.346%
3	3.958	144	148	153	rVB2	8088	12025	0.22%	0.028%
4	4.887	302	306	312	rVB7	3240	6726	0.12%	0.016%
5	6.963	652	659	673	rVB	116610	202789	3.66%	0.473%
6	7.116	679	685	697	rBV	525150	829995	14.96%	1.936%
7	7.310	710	718	729	rBV	488414	775419	13.98%	1.809%
8	7.775	788	797	806	rBV	458619	724600	13.06%	1.690%
9	8.052	840	844	848	rBV7	3588	7205	0.13%	0.017%
10	8.504	914	921	935	rBV	367679	609663	10.99%	1.422%
11	8.610	935	939	946	rVB2	15108	26945	0.49%	0.063%
12	8.940	989	995	1007	rBV	685689	1126450	20.31%	2.628%
13	9.663	1108	1118	1129	rBV	578397	959650	17.30%	2.239%
14	10.204	1202	1210	1224	rBV	787948	1345668	24.26%	3.139%
15	10.569	1264	1272	1283	rBV	637478	1032417	18.61%	2.408%
16	10.722	1290	1298	1313	rBV	562501	1005858	18.13%	2.347%
17	11.187	1372	1377	1385	rVB8	4784	10850	0.20%	0.025%
18	11.587	1441	1445	1450	rBV5	5162	8277	0.15%	0.019%
19	12.169	1537	1544	1553	rBV4	13572	28338	0.51%	0.066%
20	12.310	1563	1568	1574	rBV9	4752	8256	0.15%	0.019%
21	12.857	1655	1661	1669	rBV	32044	65783	1.19%	0.153%
22	13.322	1732	1740	1749	rBV	19562	33490	0.60%	0.078%
23	13.428	1754	1758	1765	rVB8	5324	8874	0.16%	0.021%
24	13.839	1819	1828	1839	rBV	1661779	2351920	42.40%	5.487%
25	14.116	1862	1875	1887	rBV	1844586	2623032	47.29%	6.119%
26	14.422	1918	1927	1937	rBV	1045598	1513688	27.29%	3.531%
27	14.557	1946	1950	1956	rVB9	3421	5755	0.10%	0.013%
28	14.669	1963	1969	1986	rBV	81851	190922	3.44%	0.445%
29	14.869	2000	2003	2009	rVB8	3688	6158	0.11%	0.014%
30	15.416	2087	2096	2104	rBV	2513859	3489467	62.91%	8.140%
31	15.469	2104	2105	2110	rVV5	6255	7061	0.13%	0.016%
32	15.557	2110	2120	2129	rVV	976032	1325837	23.90%	3.093%
33	15.634	2129	2133	2146	rVB3	46950	89739	1.62%	0.209%
34	16.204	2225	2230	2235	rBV4	10360	14559	0.26%	0.034%
35	16.728	2311	2319	2328	rBV4	6692	15295	0.28%	0.036%
36	16.857	2336	2341	2344	rBV5	7083	11752	0.21%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019356.D
 Acq On : 13 Jan 2024 06:35
 Operator : MA/JU
 Sample : P1091-19
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	17.180	2389	2396	2405	rBV	1399728	2015823	36.34%	4.703%
38	17.280	2406	2413	2425	rVB	3196169	4410255	79.51%	10.288%
39	17.916	2515	2521	2524	rBV5	12651	20542	0.37%	0.048%
40	18.069	2543	2547	2555	rBV2	58533	85865	1.55%	0.200%
41	18.486	2614	2618	2622	rBV6	7382	9564	0.17%	0.022%
42	18.675	2648	2650	2653	rVB4	7607	6970	0.13%	0.016%
43	19.098	2718	2722	2730	rBV2	45543	60963	1.10%	0.142%
44	19.169	2730	2734	2738	rBV	43454	62608	1.13%	0.146%
45	19.310	2754	2758	2765	rBV5	37525	53655	0.97%	0.125%
46	19.451	2780	2782	2785	rBV3	9260	8321	0.15%	0.019%
47	19.527	2788	2795	2804	rBV	4387163	5546937	100.00%	12.940%
48	21.286	3089	3094	3101	rVB	1909232	2324065	41.90%	5.422%
49	23.492	3461	3469	3479	rVB2	2690210	5379125	96.97%	12.549%
50	23.639	3487	3494	3504	rVB	1096094	2223589	40.09%	5.187%




Sum of corrected areas: 42866029

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019356.D
Acq On : 13 Jan 2024 06:35
Operator : MA/JU
Sample : P1091-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

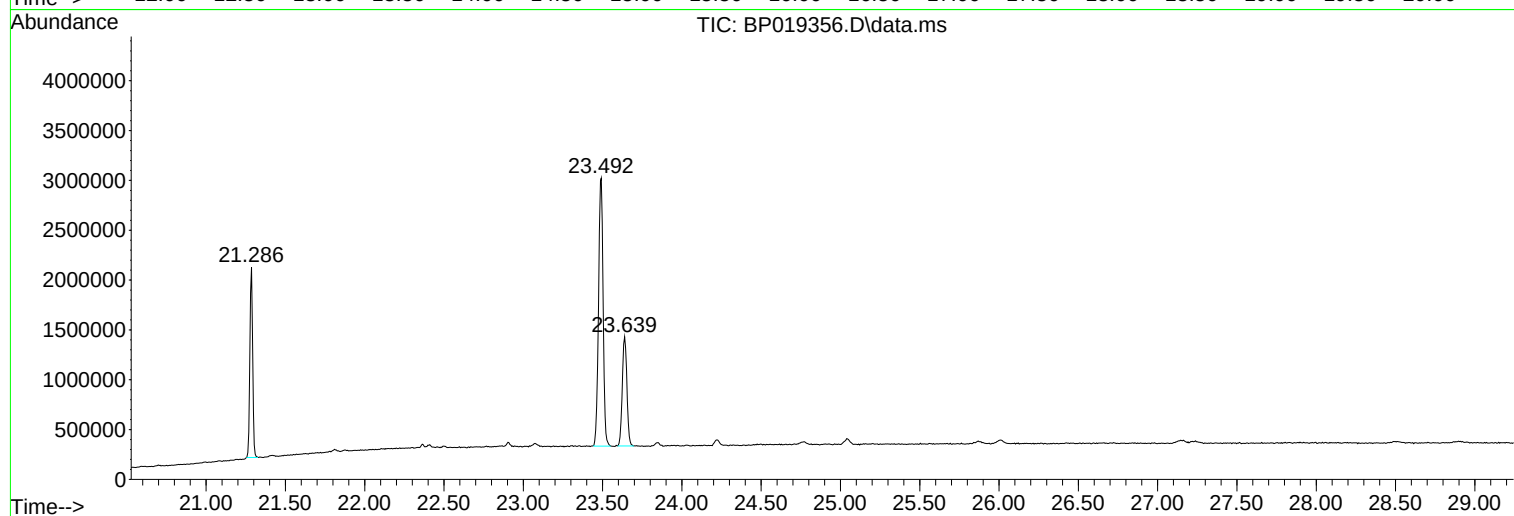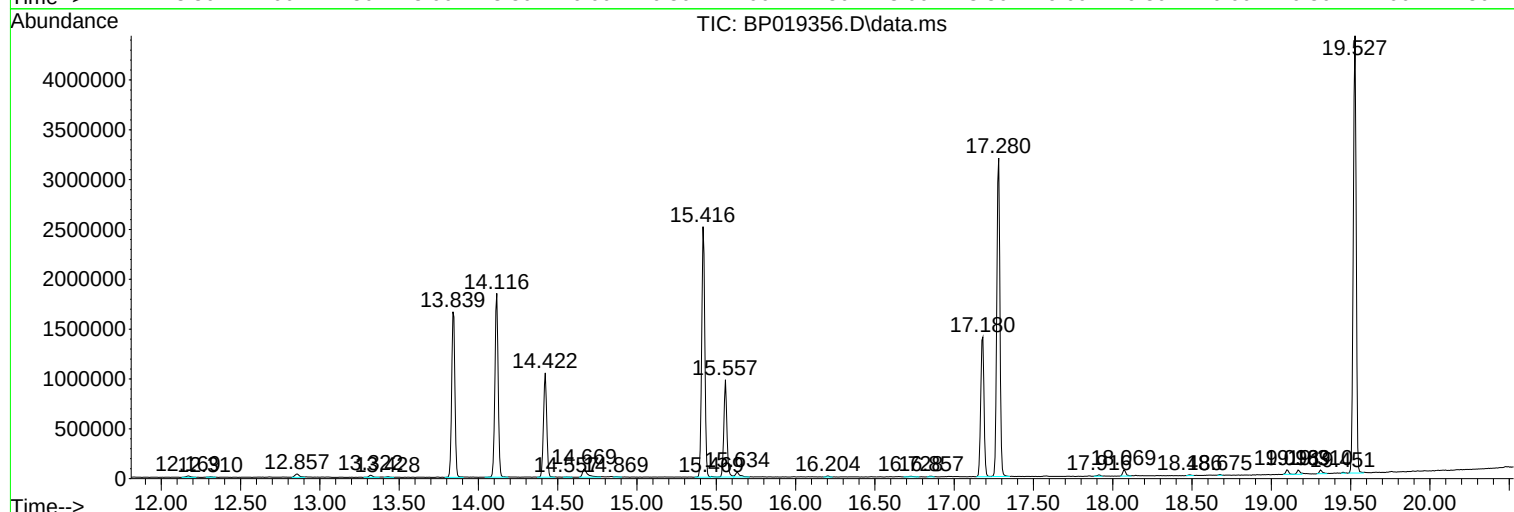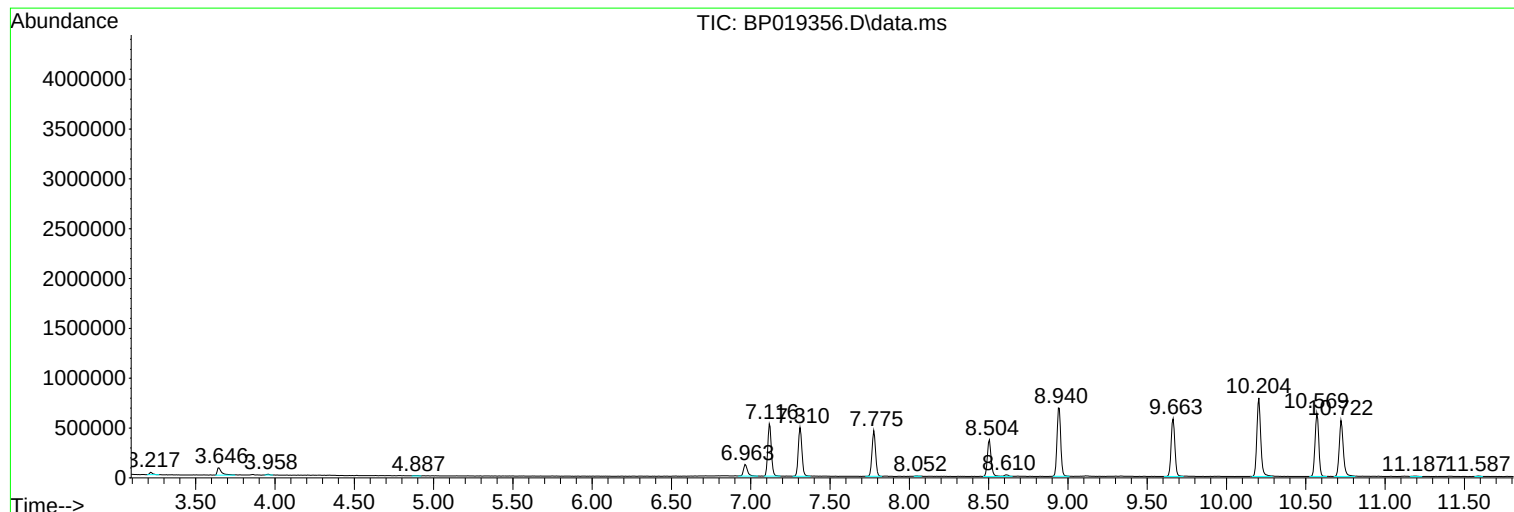

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019356.D
Acq On : 13 Jan 2024 06:35
Operator : MA/JU
Sample : P1091-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019356.D
Acq On : 13 Jan 2024 06:35
Operator : MA/JU
Sample : P1091-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc