

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019357.D
 Acq On : 13 Jan 2024 07:09
 Operator : MA/JU
 Sample : P1091-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COB03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	30	rVB	30776	45527	0.71%	0.092%
2	3.640	90	94	111	rBV	175353	291558	4.52%	0.589%
3	3.958	145	148	152	rVB2	8395	10044	0.16%	0.020%
4	6.964	653	659	672	rVB	144311	237624	3.68%	0.480%
5	7.117	678	685	699	rVB	653557	1006793	15.60%	2.032%
6	7.311	711	718	729	rBV	599688	941550	14.59%	1.901%
7	7.775	790	797	807	rVB	526869	818585	12.68%	1.652%
8	8.505	914	921	934	rBV	441230	729477	11.30%	1.473%
9	8.611	934	939	945	rVB2	10874	18114	0.28%	0.037%
10	8.946	987	996	1003	rBV	811102	1362097	21.11%	2.749%
11	9.663	1109	1118	1127	rBV	682207	1131253	17.53%	2.284%
12	10.205	1203	1210	1229	rBV	948581	1631524	25.28%	3.293%
13	10.569	1265	1272	1284	rVB	722696	1166627	18.08%	2.355%
14	10.722	1290	1298	1314	rBV	871711	1543376	23.92%	3.115%
15	12.169	1538	1544	1550	rBV3	14917	27810	0.43%	0.056%
16	13.316	1733	1739	1746	rBV4	12307	22335	0.35%	0.045%
17	13.840	1818	1828	1837	rBV	2002926	2822508	43.74%	5.697%
18	14.116	1864	1875	1888	rBV	2161098	3150871	48.83%	6.360%
19	14.422	1916	1927	1935	rBV	1138184	1680891	26.05%	3.393%
20	14.663	1961	1968	1985	rBV	103216	216488	3.35%	0.437%
21	14.869	2000	2003	2007	rVB6	5294	7546	0.12%	0.015%
22	15.416	2087	2096	2104	rBV	2903699	4219380	65.38%	8.517%
23	15.557	2113	2120	2133	rBV	1007975	1427999	22.13%	2.883%
24	15.657	2133	2137	2143	rVB2	12801	21185	0.33%	0.043%
25	16.204	2225	2230	2234	rBV3	10103	13675	0.21%	0.028%
26	16.722	2313	2318	2322	rVB8	4367	6472	0.10%	0.013%
27	16.857	2334	2341	2346	rVB8	6611	13416	0.21%	0.027%
28	16.963	2357	2359	2365	rVB6	4035	6710	0.10%	0.014%
29	17.181	2387	2396	2404	rBV	1591961	2263706	35.08%	4.569%
30	17.281	2404	2413	2427	rVV	3521068	5112658	79.23%	10.320%
31	17.398	2427	2433	2437	rVB9	6472	11533	0.18%	0.023%
32	17.569	2457	2462	2464	rBV5	6799	11307	0.18%	0.023%
33	17.851	2506	2510	2513	rBV6	4577	7089	0.11%	0.014%
34	18.069	2543	2547	2555	rBV2	64159	93976	1.46%	0.190%
35	18.487	2614	2618	2622	rVB7	9453	12922	0.20%	0.026%
36	19.098	2718	2722	2727	rVB2	51280	65020	1.01%	0.131%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019357.D
Acq On : 13 Jan 2024 07:09
Operator : MA/JU
Sample : P1091-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	19.169	2730	2734	2738	rBV	46222	64739	1.00%	0.131%
38	19.310	2754	2758	2764	rBV3	46932	66772	1.03%	0.135%
39	19.451	2780	2782	2786	rBV5	8513	8987	0.14%	0.018%
40	19.528	2788	2795	2804	rVV	4902670	6453322	100.00%	13.027%
41	21.286	3088	3094	3105	rBV	1954583	2572666	39.87%	5.193%
42	23.492	3461	3469	3479	rVB	3067455	5874820	91.04%	11.859%
43	23.639	3487	3494	3503	rVB	1180678	2348862	36.40%	4.741%



Sum of corrected areas: 49539814

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019357.D
Acq On : 13 Jan 2024 07:09
Operator : MA/JU
Sample : P1091-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

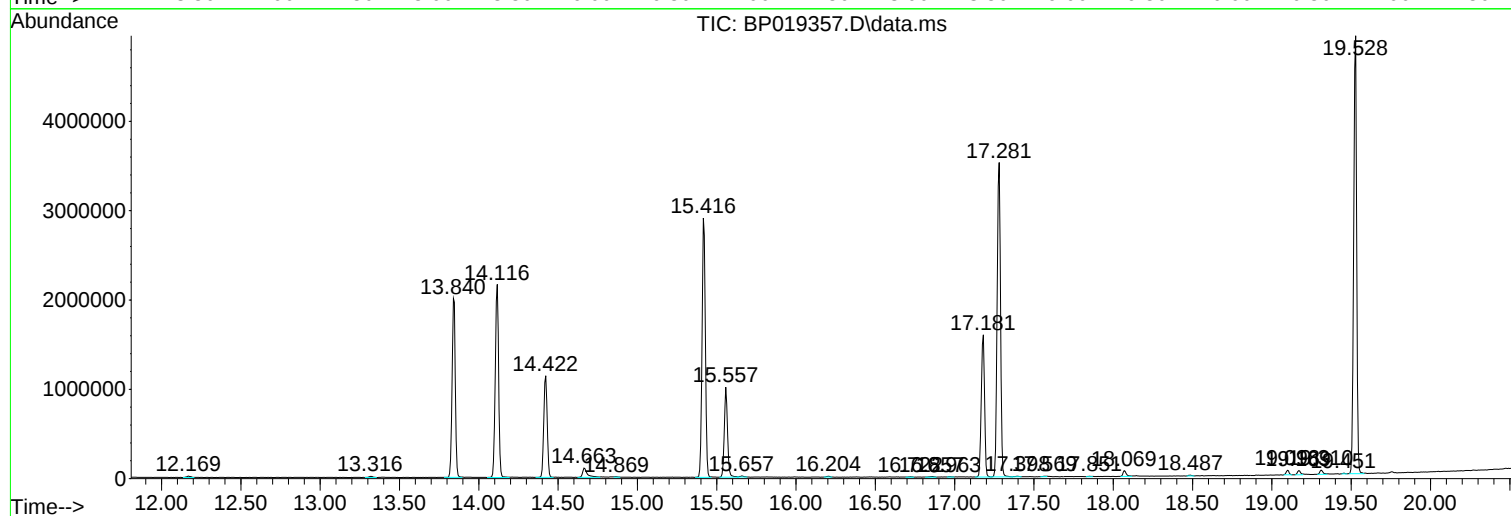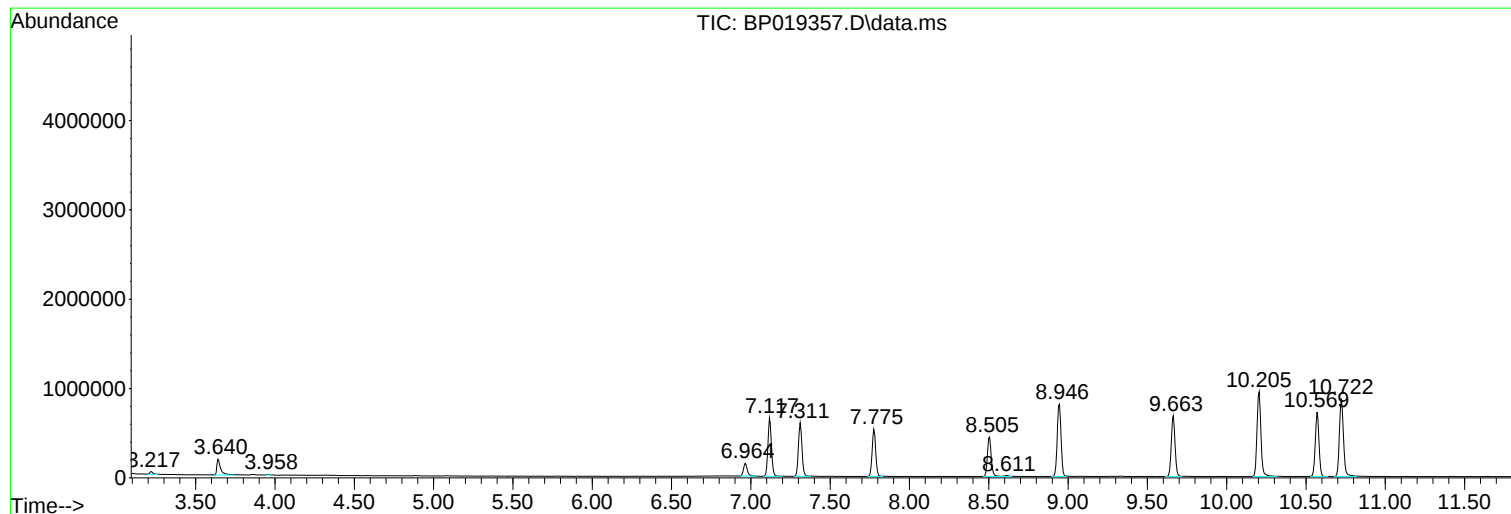

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019357.D
Acq On : 13 Jan 2024 07:09
Operator : MA/JU
Sample : P1091-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019357.D
Acq On : 13 Jan 2024 07:09
Operator : MA/JU
Sample : P1091-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc