

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019358.D
 Acq On : 13 Jan 2024 07:43
 Operator : MA/JU
 Sample : P1130-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	30	rVB	23192	34485	0.61%	0.082%
2	3.640	91	94	103	rBV	83276	141391	2.52%	0.336%
3	3.952	144	147	155	rVB3	7015	12440	0.22%	0.030%
4	6.964	653	659	670	rVB	117367	197521	3.52%	0.469%
5	7.116	679	685	696	rBV	479350	748461	13.34%	1.778%
6	7.311	711	718	729	rBV	450470	719691	12.83%	1.710%
7	7.775	787	797	805	rBV	447110	711594	12.68%	1.690%
8	8.505	913	921	931	rBV	358622	598468	10.67%	1.422%
9	8.940	988	995	1010	rBV	615228	1031300	18.38%	2.450%
10	9.334	1060	1062	1068	rVB7	4484	6168	0.11%	0.015%
11	9.663	1109	1118	1127	rBV	527896	858765	15.31%	2.040%
12	10.205	1202	1210	1228	rBV	702194	1231101	21.94%	2.924%
13	10.569	1264	1272	1282	rBV	623824	1006531	17.94%	2.391%
14	10.722	1288	1298	1317	rBV	608150	1092927	19.48%	2.596%
15	12.175	1539	1545	1552	rBV3	9822	21371	0.38%	0.051%
16	13.322	1734	1740	1746	rBV4	10148	17287	0.31%	0.041%
17	13.840	1821	1828	1839	rBV	1670437	2256285	40.21%	5.360%
18	14.116	1864	1875	1887	rBV	1682427	2430694	43.32%	5.774%
19	14.422	1918	1927	1935	rBV	1007460	1458534	25.99%	3.465%
20	14.663	1963	1968	1986	rBV	99479	218975	3.90%	0.520%
21	15.181	2052	2056	2058	rBV4	4979	6184	0.11%	0.015%
22	15.416	2088	2096	2104	rBV	2324400	3352900	59.76%	7.965%
23	15.557	2113	2120	2134	rBV	1006114	1361114	24.26%	3.233%
24	15.663	2134	2138	2144	rVB3	10936	16935	0.30%	0.040%
25	16.204	2225	2230	2234	rBV5	8612	12276	0.22%	0.029%
26	16.592	2292	2296	2301	rBV8	4152	8051	0.14%	0.019%
27	16.857	2338	2341	2345	rVB5	4522	5805	0.10%	0.014%
28	17.181	2389	2396	2404	rBV	1407276	1961296	34.96%	4.659%
29	17.281	2405	2413	2423	rBV	3091471	4400345	78.43%	10.453%
30	18.069	2543	2547	2556	rBV3	70599	108096	1.93%	0.257%
31	18.481	2615	2617	2622	rVB6	6733	7689	0.14%	0.018%
32	19.098	2718	2722	2727	rBV2	44843	58210	1.04%	0.138%
33	19.169	2730	2734	2741	rBV2	42325	69881	1.25%	0.166%
34	19.310	2754	2758	2764	rBV4	29160	45461	0.81%	0.108%
35	19.528	2788	2795	2807	rBV	4152538	5591677	99.66%	13.283%
36	20.992	3041	3044	3050	rBV6	46692	73907	1.32%	0.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019358.D
Acq On : 13 Jan 2024 07:43
Operator : MA/JU
Sample : P1130-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	21.286	3088	3094	3102	rBV	1810703	2339393	41.69%	5.557%
38	23.486	3461	3468	3482	rVB2	2912402	5610848	100.00%	13.328%
39	23.639	3487	3494	3502	rVB	1138286	2273856	40.53%	5.401%




Sum of corrected areas: 42097913

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019358.D
Acq On : 13 Jan 2024 07:43
Operator : MA/JU
Sample : P1130-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

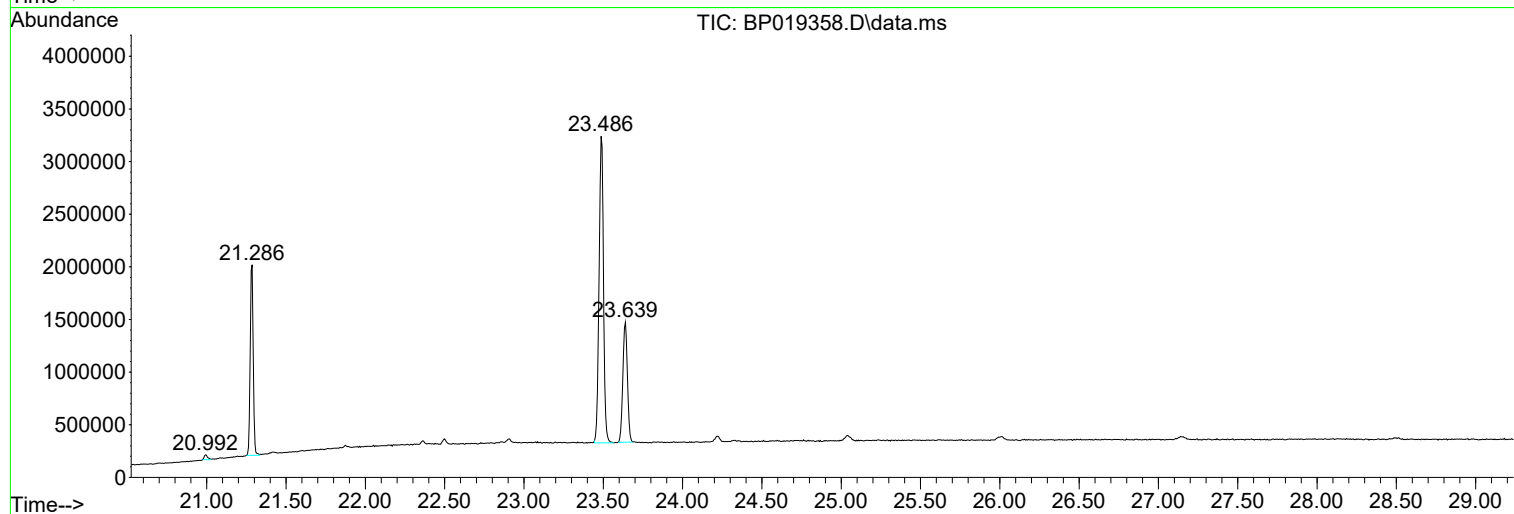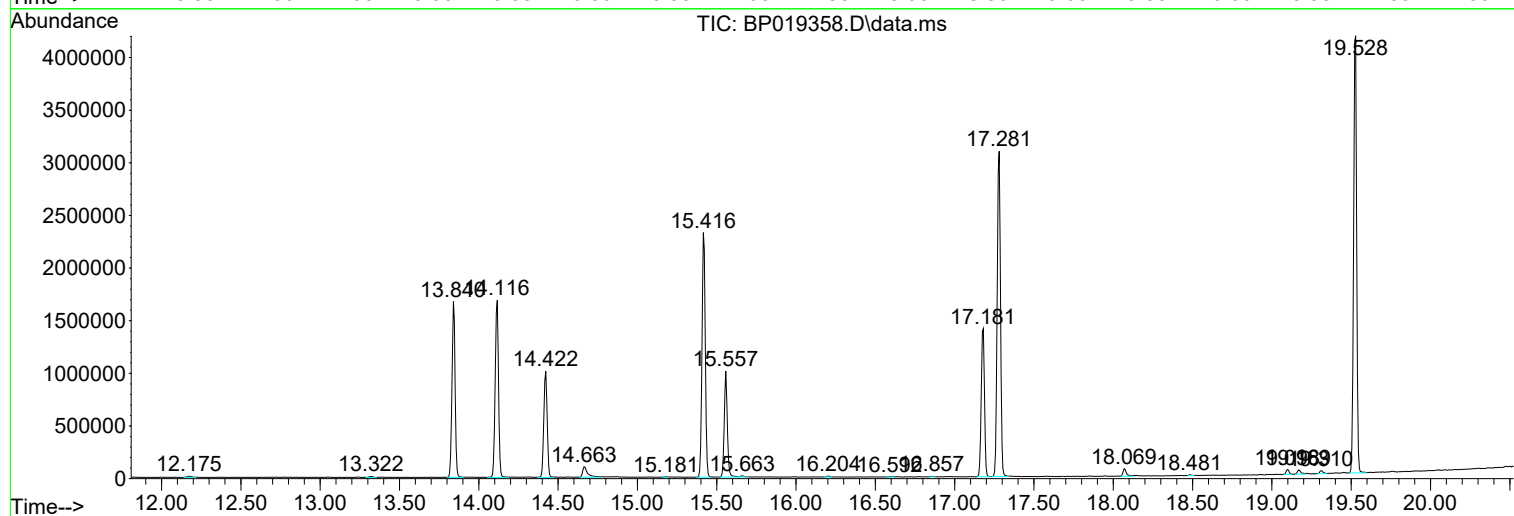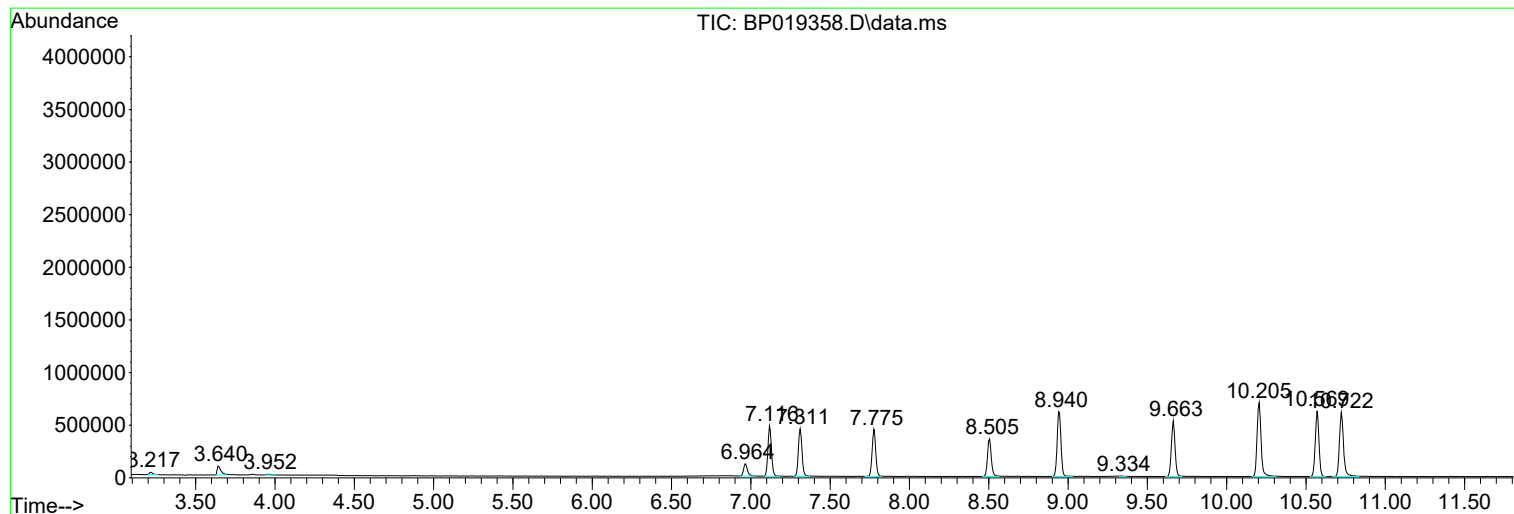

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019358.D
Acq On : 13 Jan 2024 07:43
Operator : MA/JU
Sample : P1130-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019358.D
Acq On : 13 Jan 2024 07:43
Operator : MA/JU
Sample : P1130-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc