

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
 Data File : BP019359.D
 Acq On : 13 Jan 2024 08:17
 Operator : MA/JU
 Sample : P1130-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	28	rBV	22692	32215	0.60%	0.078%
2	3.640	90	94	108	rBV	105282	187142	3.50%	0.452%
3	3.952	145	147	157	rVB2	7749	11960	0.22%	0.029%
4	6.963	654	659	668	rVB	105740	183653	3.44%	0.443%
5	7.116	680	685	698	rVB	513923	803436	15.03%	1.940%
6	7.310	710	718	731	rBV	469583	747966	13.99%	1.806%
7	7.775	789	797	806	rBV	456846	718043	13.43%	1.734%
8	8.504	914	921	935	rBV	342370	578594	10.83%	1.397%
9	8.946	987	996	1004	rBV	651408	1086614	20.33%	2.624%
10	9.334	1057	1062	1067	rVB9	4563	9829	0.18%	0.024%
11	9.663	1108	1118	1128	rBV	556531	908991	17.01%	2.195%
12	10.204	1201	1210	1228	rBV	723553	1282725	24.00%	3.097%
13	10.569	1264	1272	1283	rVB	617468	1016258	19.01%	2.454%
14	10.722	1291	1298	1311	rBV	599340	1080999	20.22%	2.610%
15	12.175	1539	1545	1554	rVB2	11543	24359	0.46%	0.059%
16	13.240	1722	1726	1730	rVB5	3675	5392	0.10%	0.013%
17	13.322	1730	1740	1745	rBV3	12727	21667	0.41%	0.052%
18	13.840	1821	1828	1838	rBV	1640824	2242037	41.95%	5.413%
19	14.116	1867	1875	1889	rBV	1755516	2484144	46.48%	5.998%
20	14.422	1920	1927	1936	rBV	985423	1445061	27.04%	3.489%
21	14.669	1960	1969	1984	rBV2	75558	181696	3.40%	0.439%
22	14.845	1992	1999	2003	rBV10	2906	5508	0.10%	0.013%
23	15.416	2087	2096	2104	rBV	2343553	3321727	62.15%	8.020%
24	15.557	2113	2120	2133	rBV	936573	1292923	24.19%	3.122%
25	15.663	2133	2138	2143	rVB2	10788	18955	0.35%	0.046%
26	16.204	2225	2230	2235	rVB5	9403	13527	0.25%	0.033%
27	16.592	2290	2296	2302	rBV9	5949	12669	0.24%	0.031%
28	16.851	2336	2340	2346	rBV9	5091	7681	0.14%	0.019%
29	16.963	2356	2359	2362	rBV4	3890	5780	0.11%	0.014%
30	17.181	2389	2396	2404	rBV	1369131	1940012	36.30%	4.684%
31	17.281	2406	2413	2424	rBV2	2837066	4111091	76.92%	9.926%
32	17.580	2461	2464	2470	rVB8	4544	7498	0.14%	0.018%
33	17.945	2523	2526	2531	rBV7	5668	8629	0.16%	0.021%
34	18.069	2543	2547	2554	rBV	94967	137479	2.57%	0.332%
35	18.480	2615	2617	2621	rVB4	5708	6042	0.11%	0.015%
36	19.098	2718	2722	2728	rBV	43162	59212	1.11%	0.143%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019359.D
Acq On : 13 Jan 2024 08:17
Operator : MA/JU
Sample : P1130-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	19.169	2730	2734	2741	rBV	41471	67792	1.27%	0.164%
38	19.310	2754	2758	2766	rBV3	55935	87854	1.64%	0.212%
39	19.527	2789	2795	2805	rBV	3978023	5235733	97.96%	12.642%
40	20.992	3041	3044	3051	rBV6	53987	83871	1.57%	0.203%
41	21.286	3088	3094	3101	rBV	1780705	2329258	43.58%	5.624%
42	23.486	3461	3468	3481	rVB2	2611102	5344932	100.00%	12.906%
43	23.639	3487	3494	3505	rVB	1124401	2264836	42.37%	5.469%




Sum of corrected areas: 41415790

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019359.D
Acq On : 13 Jan 2024 08:17
Operator : MA/JU
Sample : P1130-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

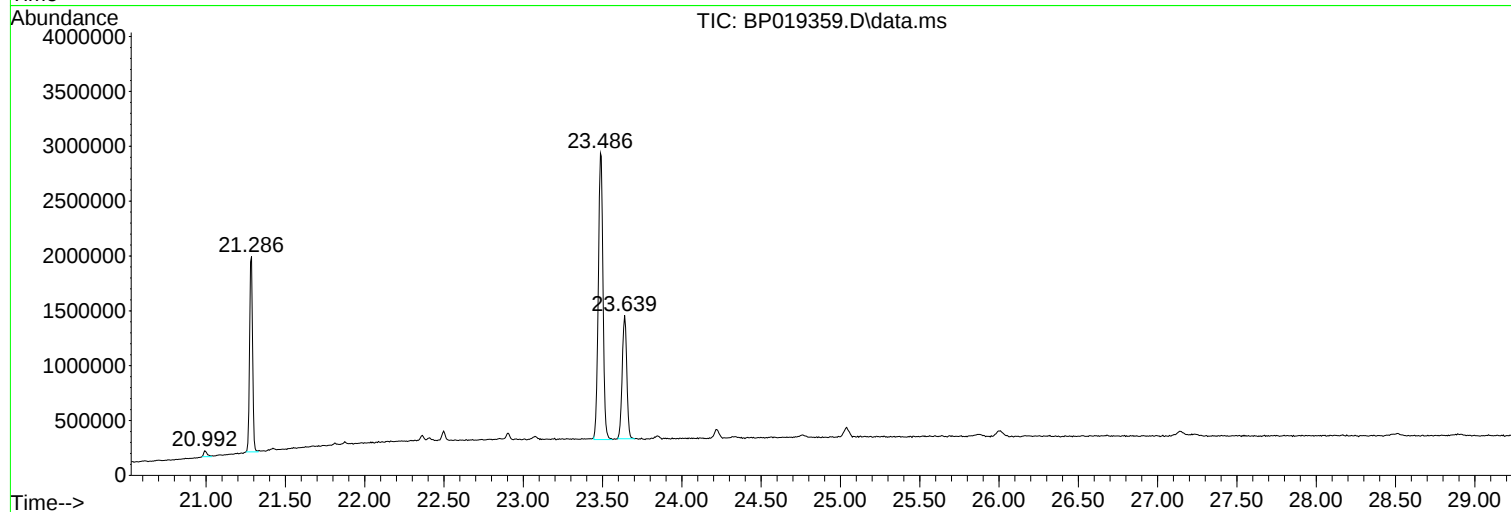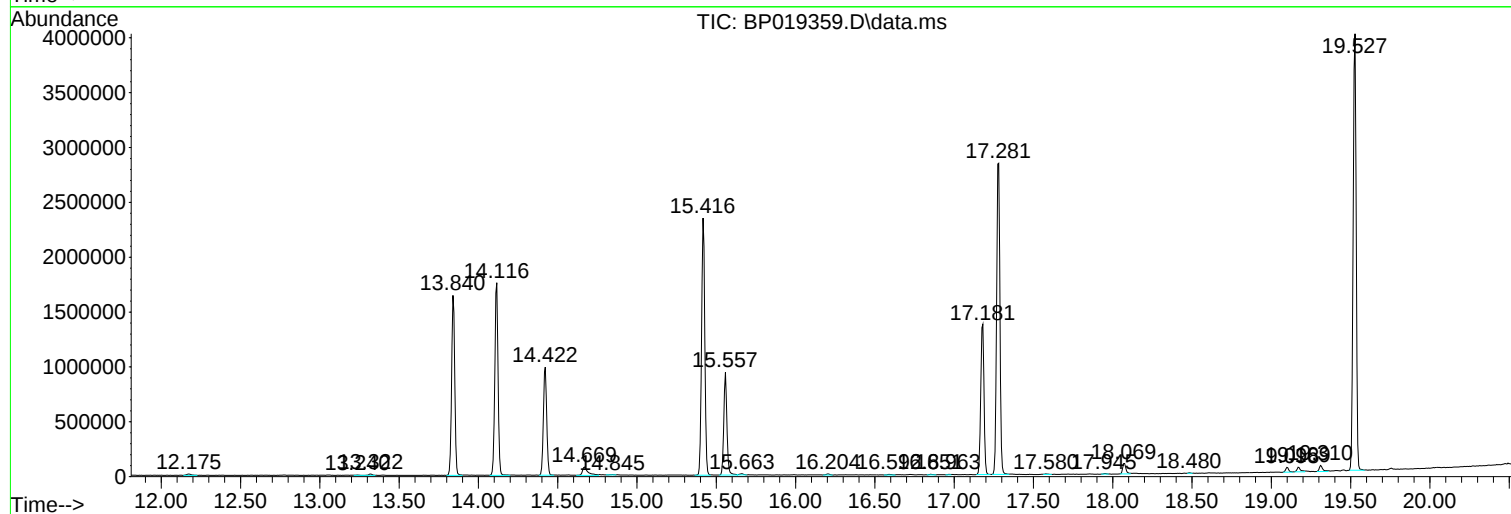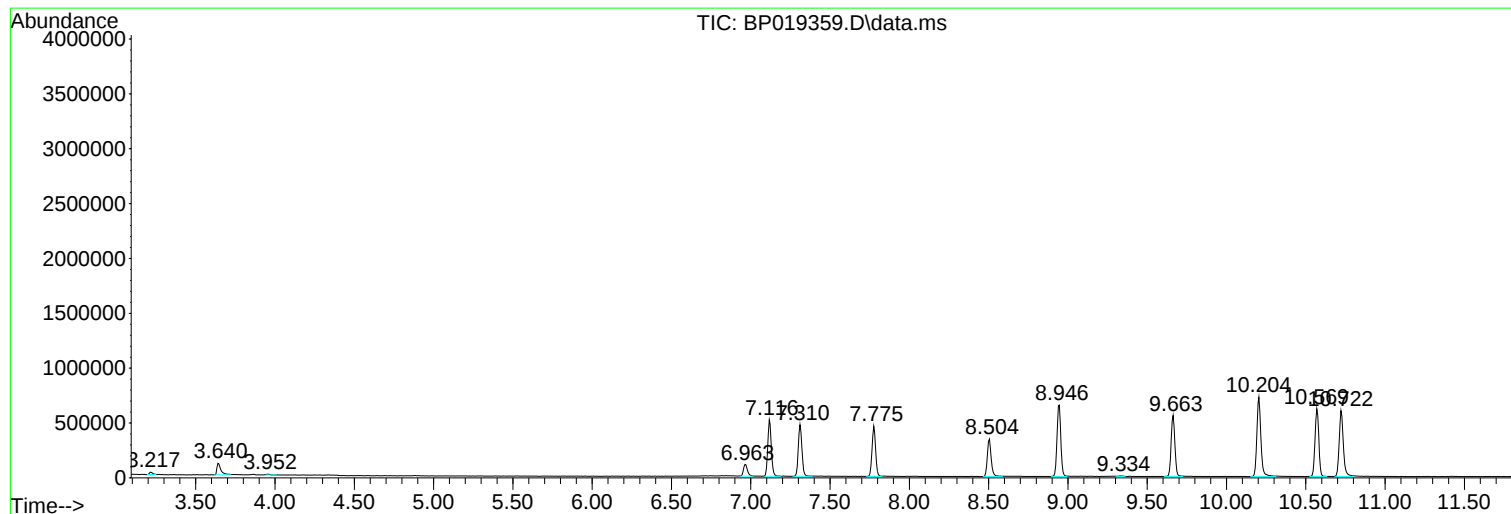

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019359.D
Acq On : 13 Jan 2024 08:17
Operator : MA/JU
Sample : P1130-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011224\
Data File : BP019359.D
Acq On : 13 Jan 2024 08:17
Operator : MA/JU
Sample : P1130-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------