

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011321\
 Data File : BP004547.D
 Acq On : 13 Jan 2021 20:37
 Operator : CG/JU
 Sample : M1091-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-03-011221

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	371	377	386	rBV	378366	573140	15.11%	2.624%
2	6.987	639	646	664	rBV	332598	597125	15.74%	2.734%
3	7.816	777	787	797	rBV	699681	1146097	30.22%	5.247%
4	8.969	977	983	991	rBV	206762	363594	9.59%	1.665%
5	10.610	1250	1262	1276	rBV	885573	1539173	40.58%	7.046%
6	13.081	1672	1682	1694	rBV	693057	1038268	27.37%	4.753%
7	13.916	1819	1824	1829	rBV	58170	80406	2.12%	0.368%
8	14.463	1910	1917	1926	rBV	1363230	2154726	56.81%	9.864%
9	15.963	2166	2172	2189	rBV	571891	900850	23.75%	4.124%
10	16.192	2207	2211	2221	rVB3	29881	57817	1.52%	0.265%
11	17.228	2381	2387	2392	rBV	1928877	2785117	73.43%	12.750%
12	17.269	2392	2394	2401	rVB	120641	147619	3.89%	0.676%
13	17.363	2406	2410	2415	rVB	44706	65959	1.74%	0.302%
14	18.116	2532	2538	2540	rBV2	36615	84796	2.24%	0.388%
15	18.286	2563	2567	2571	rBV3	53269	95482	2.52%	0.437%
16	18.404	2584	2587	2590	rBV	42675	46901	1.24%	0.215%
17	18.992	2683	2687	2689	rBV	86936	134835	3.55%	0.617%
18	19.245	2726	2730	2737	rBV	197967	269463	7.10%	1.234%
19	19.575	2783	2786	2787	rBV2	94861	105051	2.77%	0.481%
20	19.598	2787	2790	2798	rVB	215101	356808	9.41%	1.633%
21	19.792	2818	2823	2827	rBV	1570173	1866277	49.20%	8.544%
22	21.322	3078	3083	3088	rBV	2781859	3641266	96.00%	16.670%
23	23.680	3478	3484	3493	rVB2	1876486	3793092	100.00%	17.365%




Sum of corrected areas: 21843862

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011321\
Data File : BP004547.D
Acq On : 13 Jan 2021 20:37
Operator : CG/JU
Sample : M1091-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-011221

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

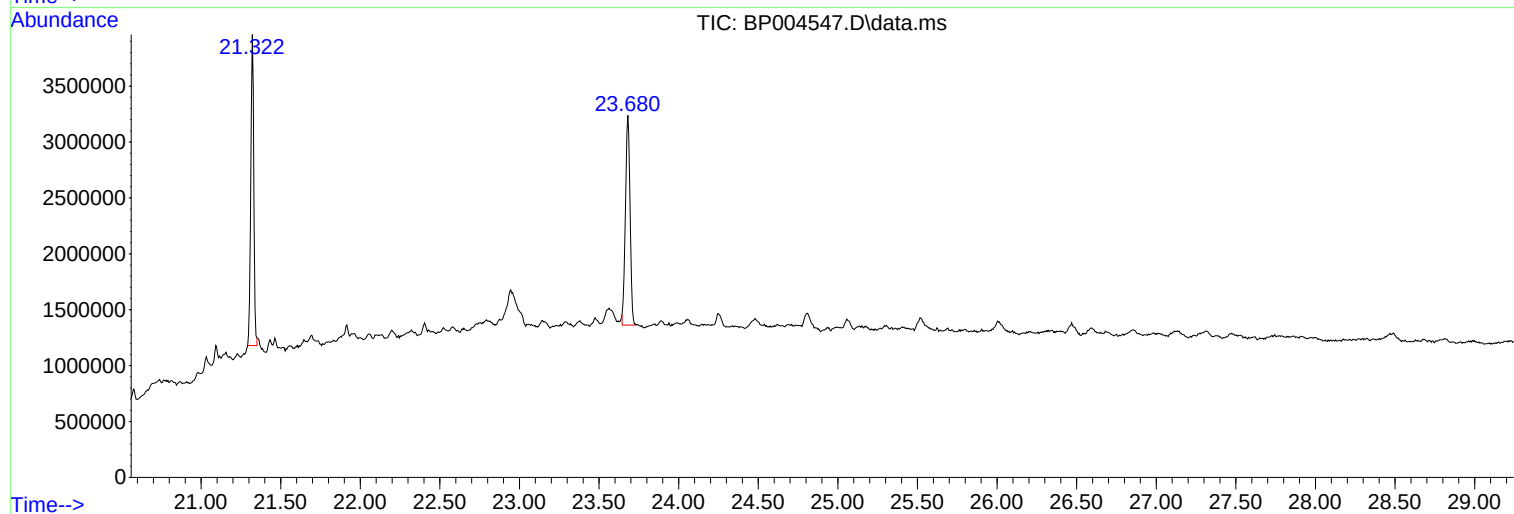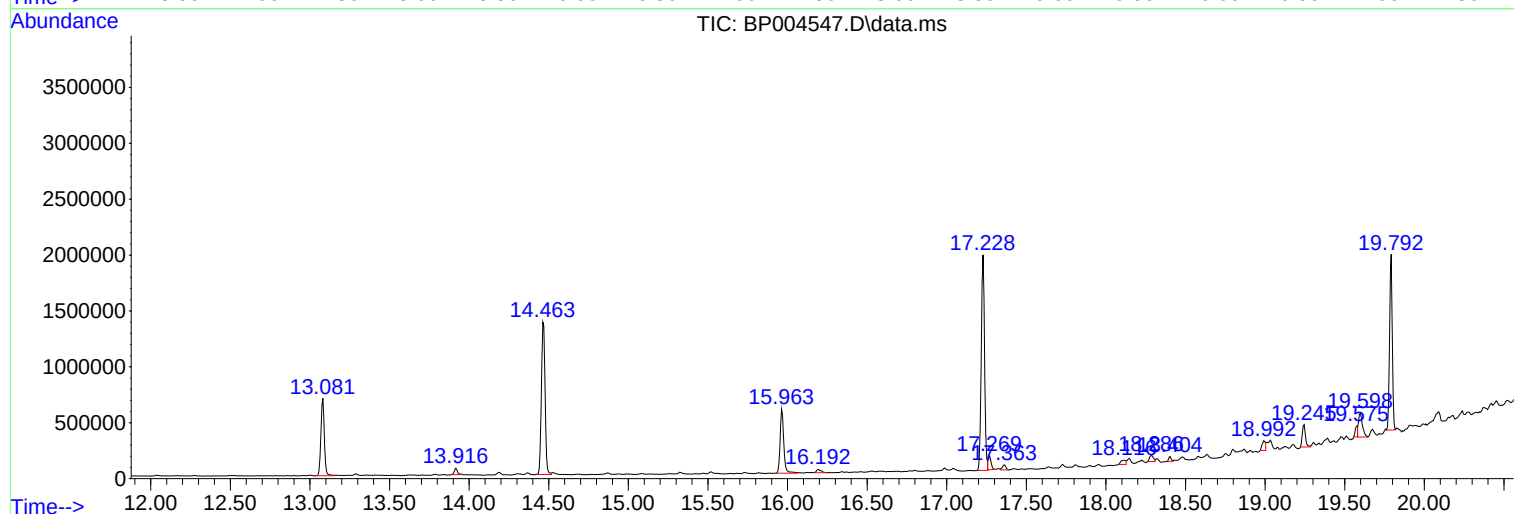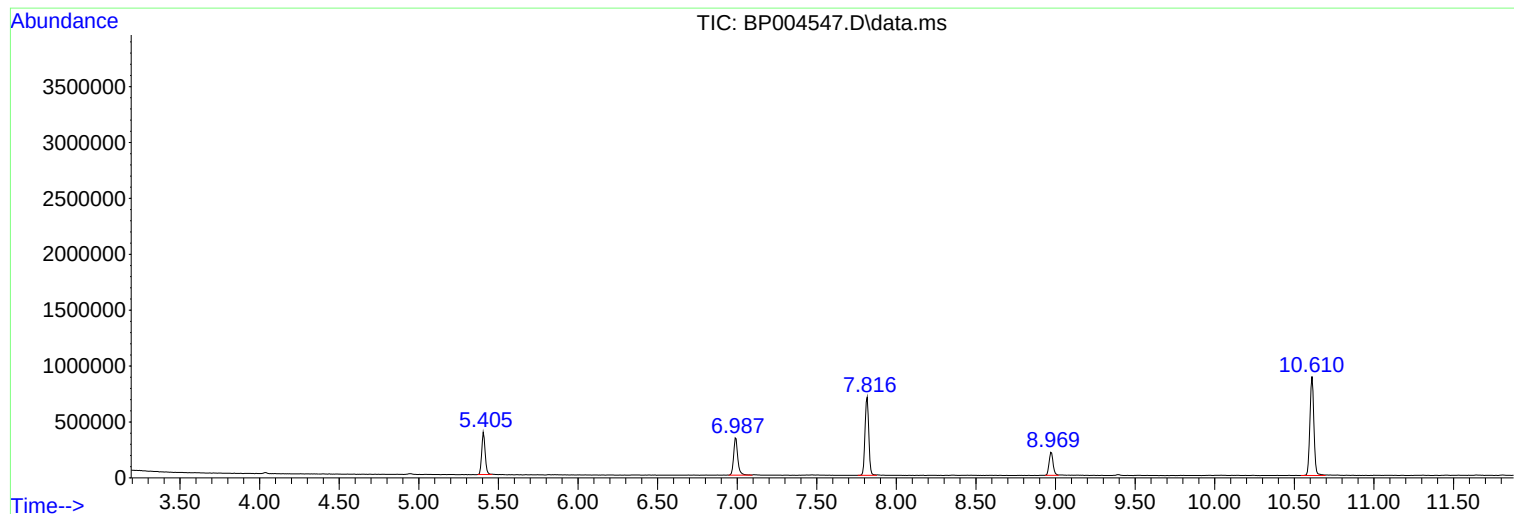

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011321\
Data File : BP004547.D
Acq On : 13 Jan 2021 20:37
Operator : CG/JU
Sample : M1091-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-011221

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011321\
Data File : BP004547.D
Acq On : 13 Jan 2021 20:37
Operator : CG/JU
Sample : M1091-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-011221

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc