
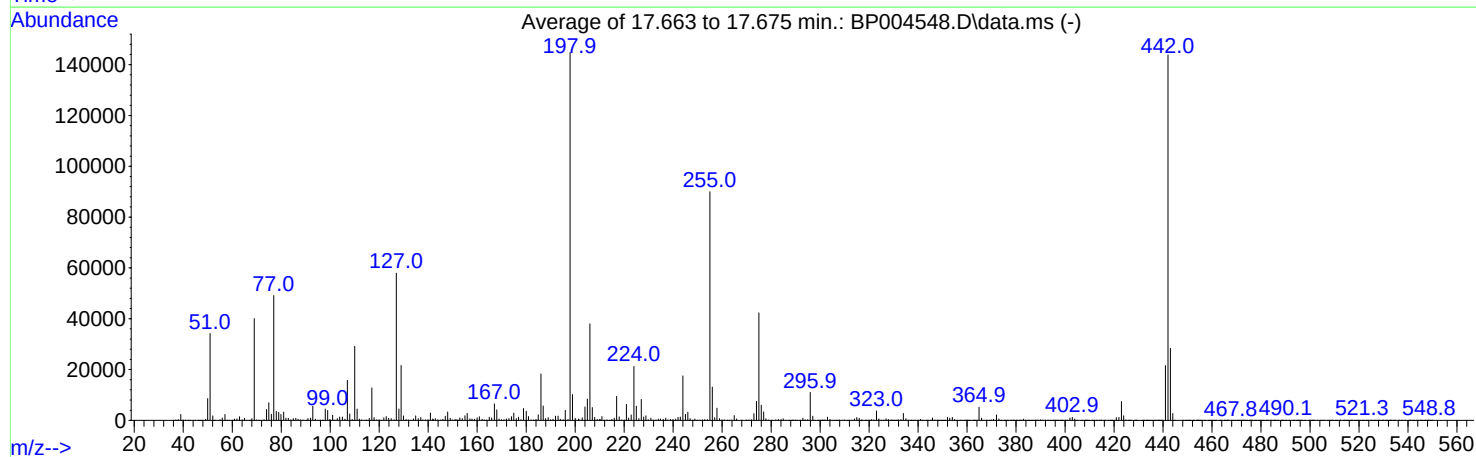


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP011421\  
 Data File : BP004548.D  
 Acq On : 14 Jan 2021 09:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270E-BP011221.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jan 12 15:19:32 2021

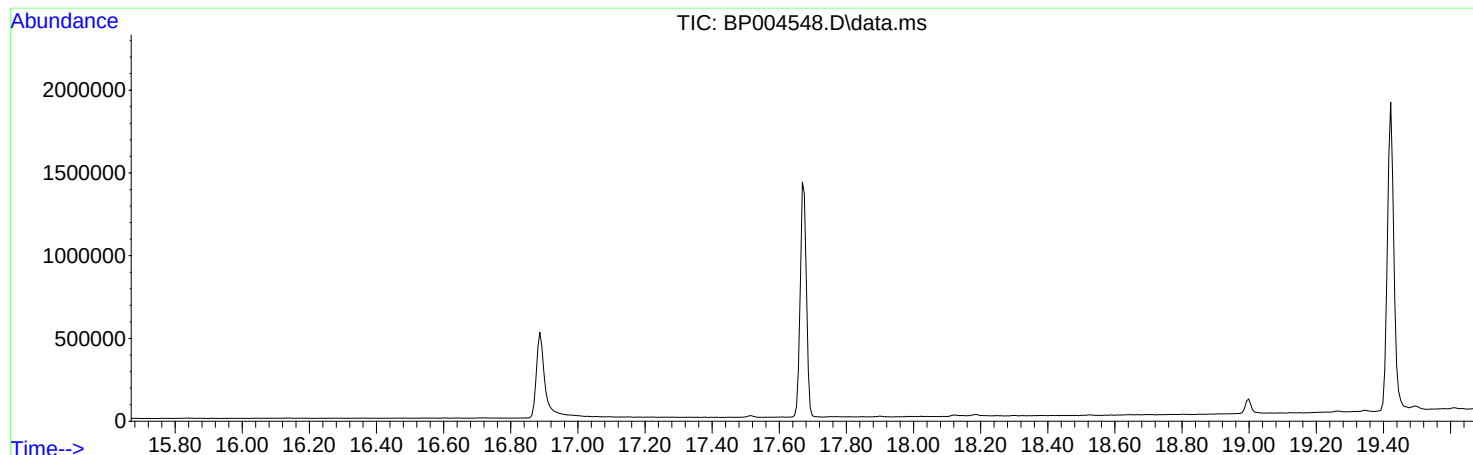

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2450

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 23.6         | 34225      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 680        | PASS                |
| 69             | 198             | 0.00            | 100             | 27.7         | 40064      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 208        | PASS                |
| 127            | 198             | 10              | 80              | 40.0         | 57971      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 397        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 144788     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 10169      | PASS                |
| 275            | 198             | 10              | 60              | 29.2         | 42314      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 5177       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.9         | 21601      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 143819     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 28356      | PASS                |