

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
 Data File : BP008814.D
 Acq On : 14 Jan 2022 18:53
 Operator : CG/JU
 Sample : PB142011BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142011BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	30	rVB	262892	365817	1.87%	0.397%
2	5.440	410	417	444	rBV	6095810	9400085	48.11%	10.195%
3	7.034	680	688	712	rBV	5592297	9361794	47.91%	10.153%
4	7.858	820	828	839	rBV	1280806	2134567	10.92%	2.315%
5	9.016	1016	1025	1047	rBV	3546592	6196365	31.71%	6.720%
6	10.657	1294	1304	1322	rBV	1606457	2862090	14.65%	3.104%
7	13.122	1714	1723	1747	rBV	10184065	15833902	81.03%	17.172%
8	14.492	1949	1956	1971	rBV	2539650	3877511	19.84%	4.205%
9	15.987	2203	2210	2239	rBV	7365811	11405814	58.37%	12.370%
10	17.251	2417	2425	2439	rBV	2839379	4381383	22.42%	4.752%
11	19.810	2854	2860	2874	rBV	15422508	19540120	100.00%	21.192%
12	21.122	3080	3083	3087	rBV	179191	307541	1.57%	0.334%
13	21.339	3115	3120	3129	rBV	2668319	3398053	17.39%	3.685%
14	21.457	3137	3140	3145	rBV	138597	203284	1.04%	0.220%
15	23.763	3525	3532	3543	rVB2	1395047	2937783	15.03%	3.186%

Sum of corrected areas: 92206109

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
Data File : BP008814.D
Acq On : 14 Jan 2022 18:53
Operator : CG/JU
Sample : PB142011BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142011BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.064	3.43 ng	365817	1,4-Dichlorobenzene-d4	7.858

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

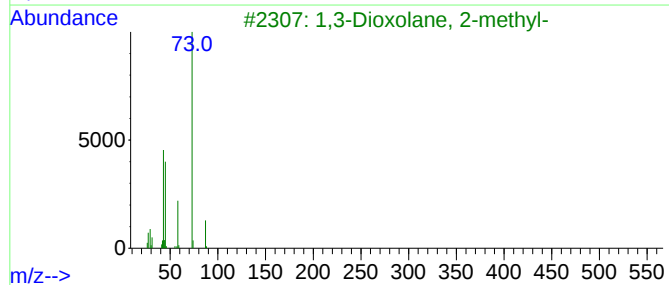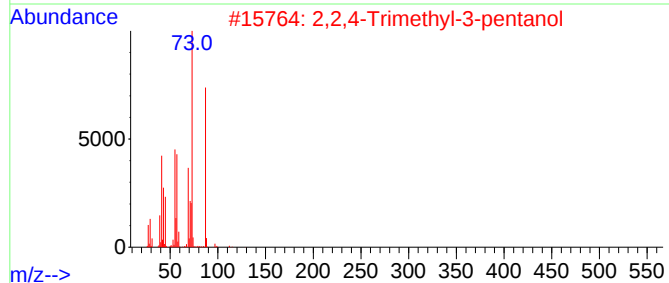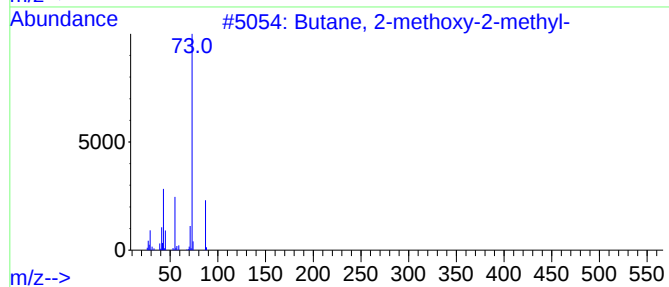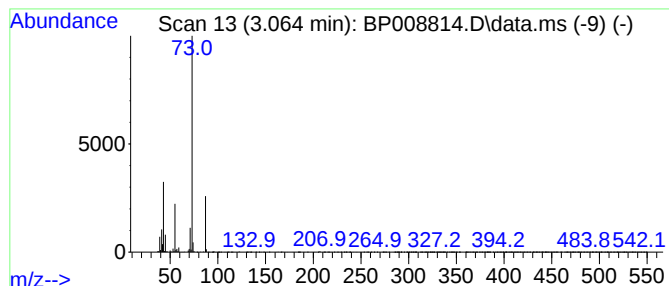

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
Data File : BP008814.D
Acq On : 14 Jan 2022 18:53
Operator : CG/JU
Sample : PB142011BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142011BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.064	3.4	ng	365817	1	7.858	2134570	20.0