
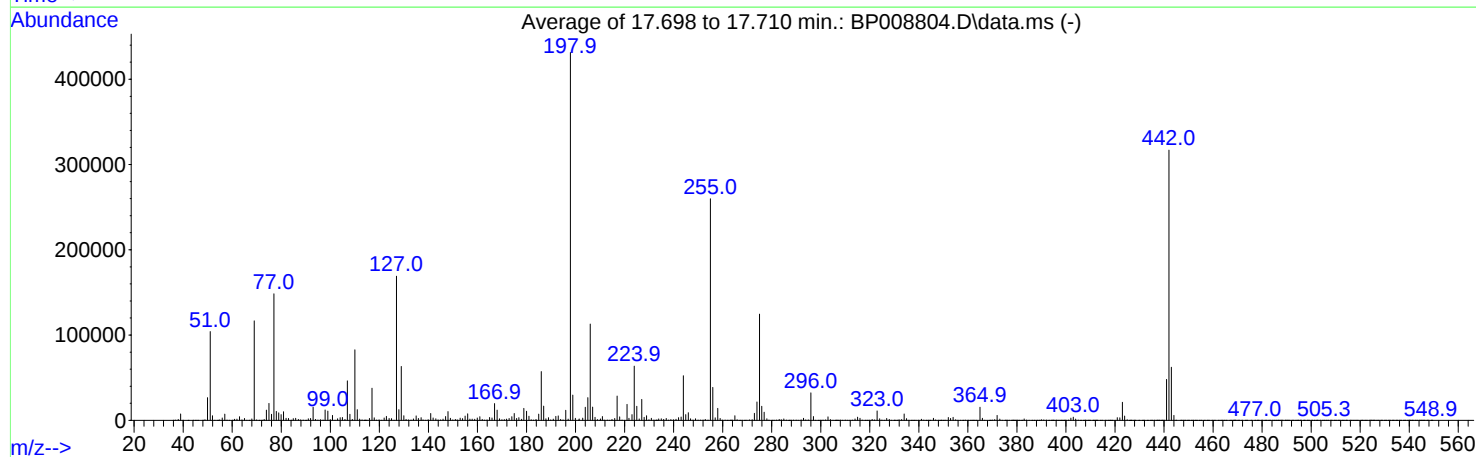


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
 Data File : BP008804.D
 Acq On : 14 Jan 2022 12:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 18:05:00 2022

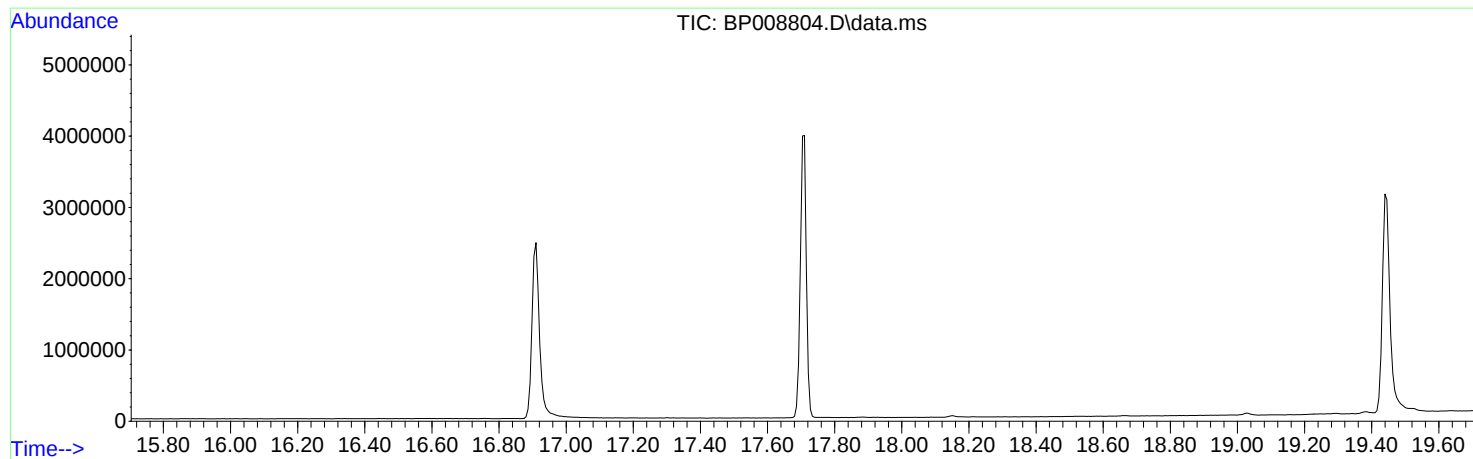




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	104208	PASS
68	69	0.00	2	1.4	1680	PASS
69	198	0.00	100	27.1	116716	PASS
70	69	0.00	2	0.5	598	PASS
127	198	10	80	39.2	169137	PASS
197	198	0.00	2	0.4	1590	PASS
198	198	100	100	100.0	431342	PASS
199	198	5	9	6.9	29603	PASS
275	198	10	60	28.9	124669	PASS
365	198	1	100	3.6	15400	PASS
441	198	0.01	100	11.1	47952	PASS
442	442	100	100	100.0	316965	PASS
443	442	15	24	19.7	62325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
Data File : BP008804.D
Acq On : 14 Jan 2022 12:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 17 05:22:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

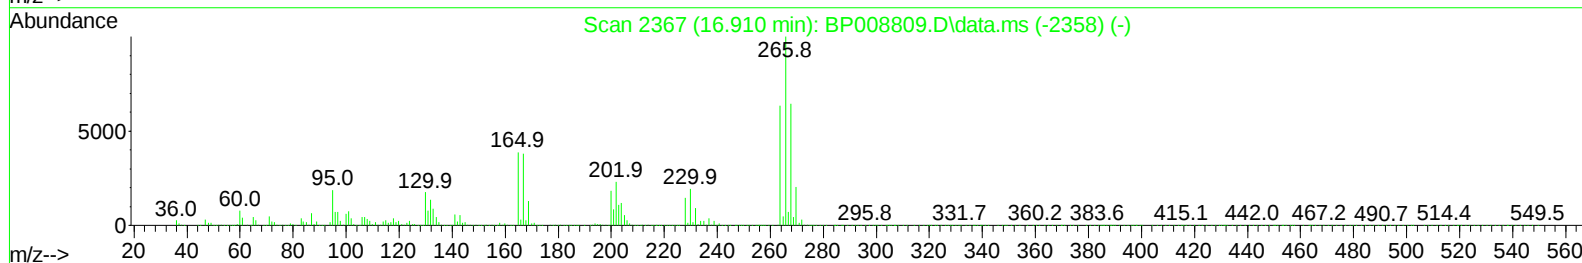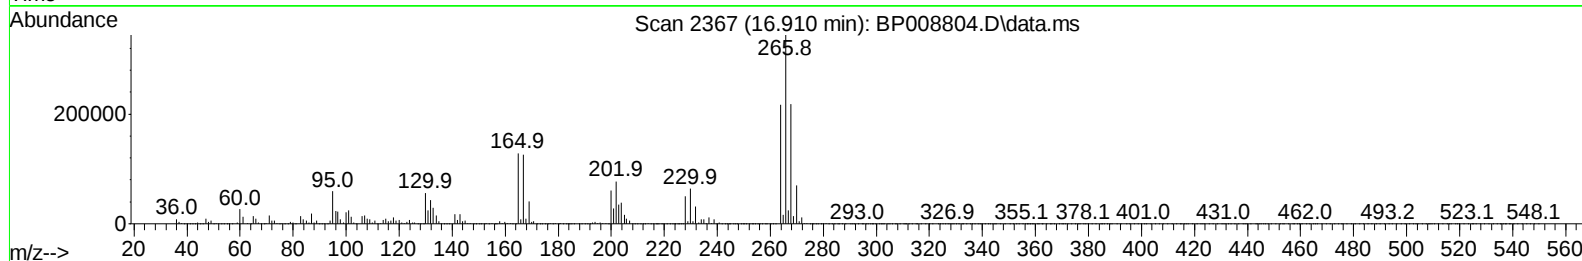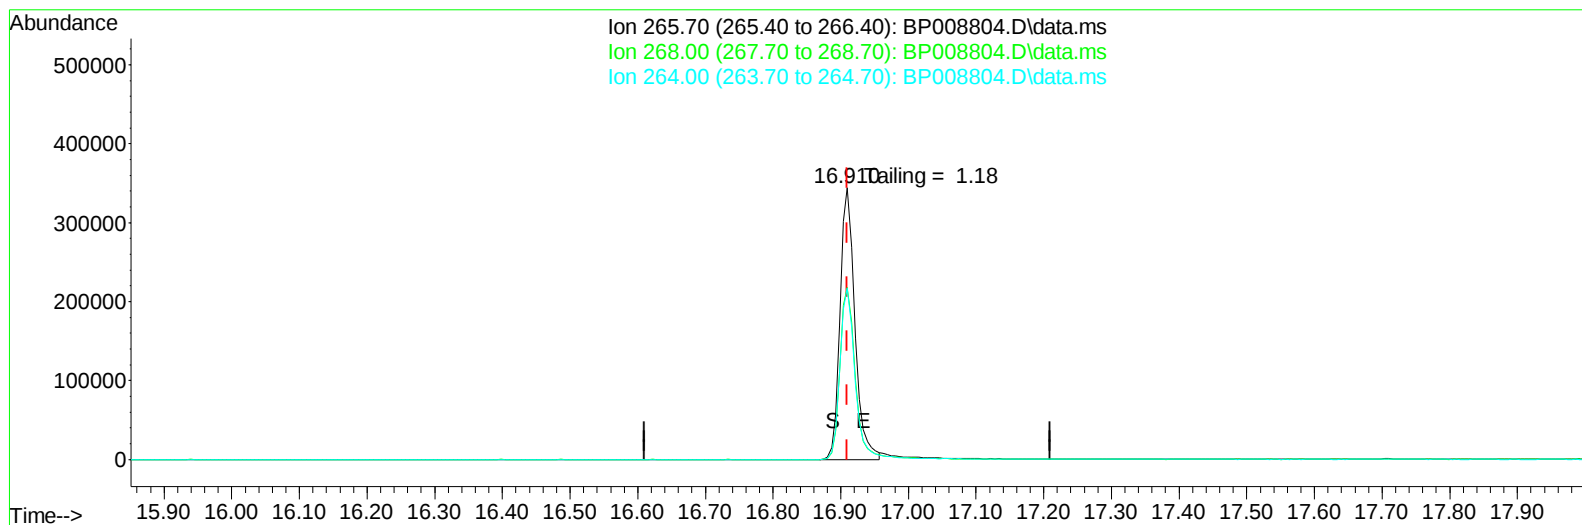

TIC: BP008804.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 207100.91 ng




response 535110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.40
264.00	62.90	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011422\
Data File : BP008804.D
Acq On : 14 Jan 2022 12:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 17 05:22:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

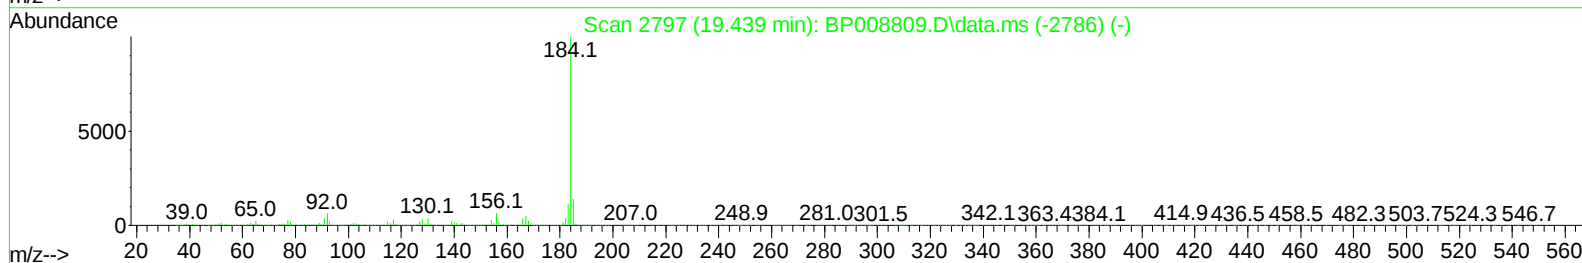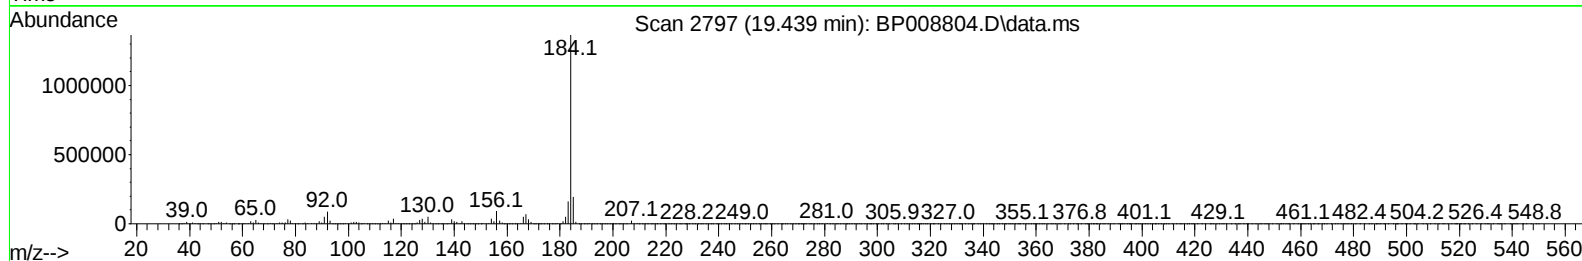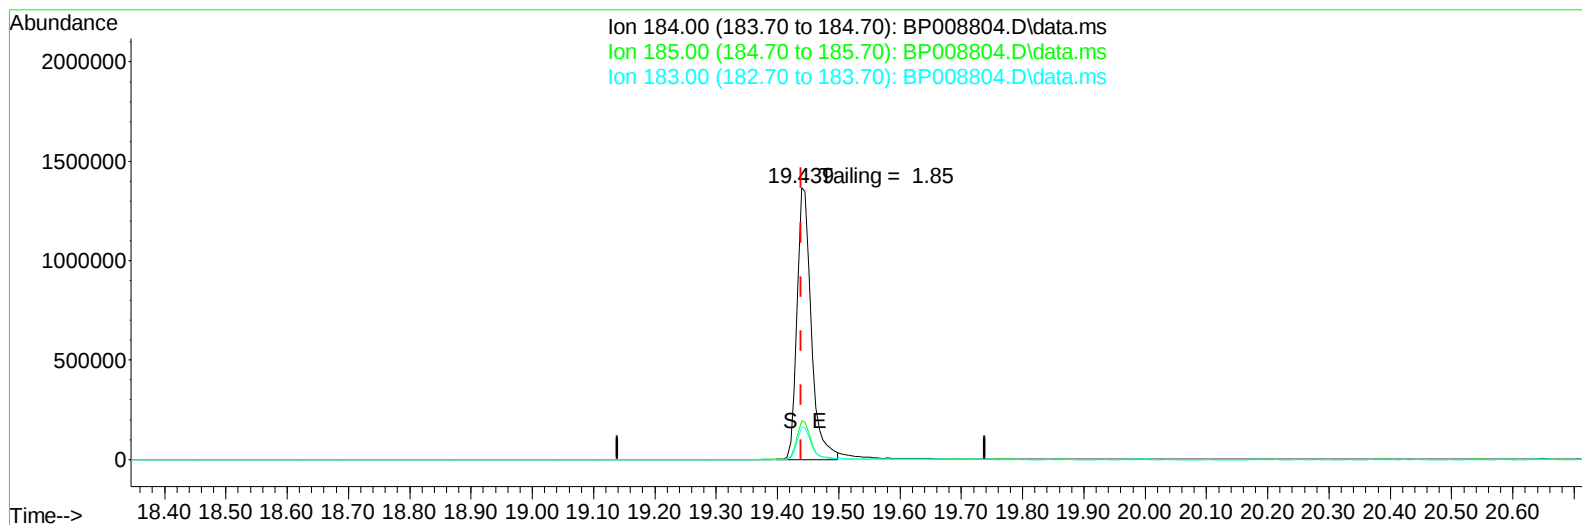

TIC: BP008804.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 52697.54 ng

response 2293599

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.33
183.00	11.90	12.04
0.00	0.00	0.00

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/14/2022	BNA_P	<u>BP008804.D</u>
Compound Name	Response	Retention Time
DDT	1317600	20.65
DDD	20092	20.22
DDE	2138	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22230	1339830	1.66