
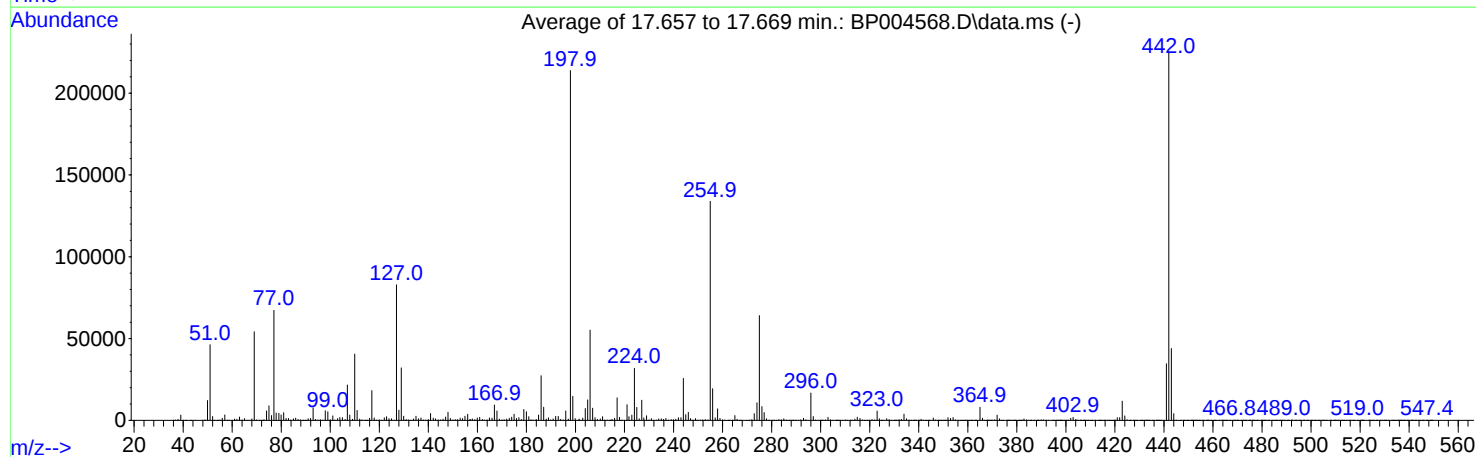


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011521\
 Data File : BP004568.D
 Acq On : 15 Jan 2021 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 12 15:19:32 2021

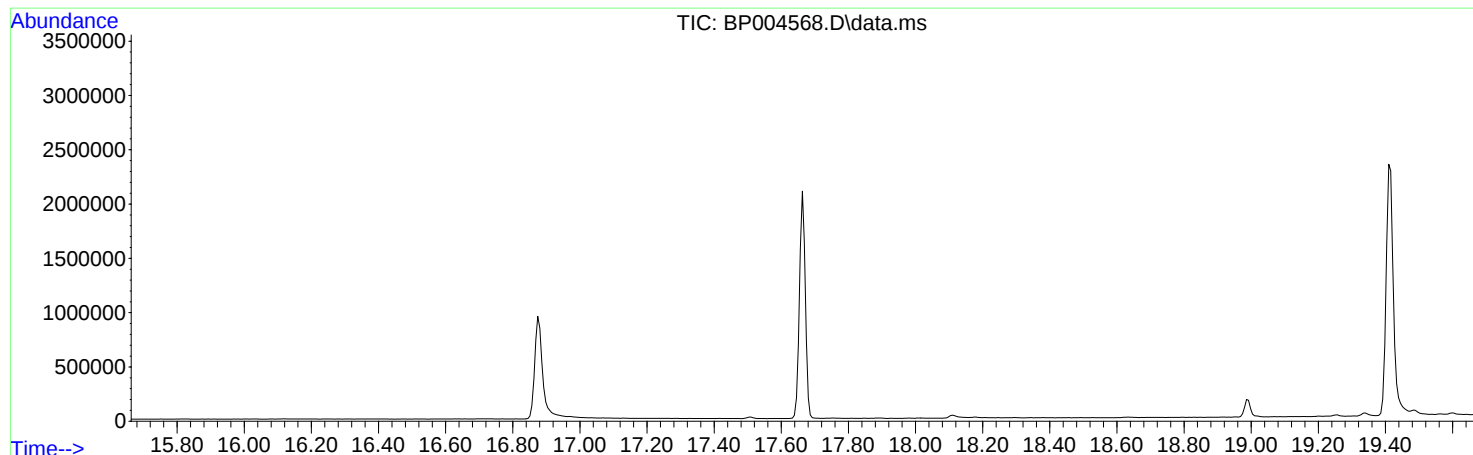

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	46307	PASS
68	69	0.00	2	1.6	876	PASS
69	198	0.00	100	25.4	54217	PASS
70	69	0.00	2	0.6	307	PASS
127	198	10	80	38.7	82800	PASS
197	198	0.00	2	0.4	820	PASS
198	198	100	100	100.0	213855	PASS
199	198	5	9	6.9	14720	PASS
275	198	10	60	30.0	64104	PASS
365	198	1	100	3.8	8043	PASS
441	198	0.01	100	16.2	34621	PASS
442	442	100	100	100.0	224853	PASS
443	442	15	24	19.5	43928	PASS