
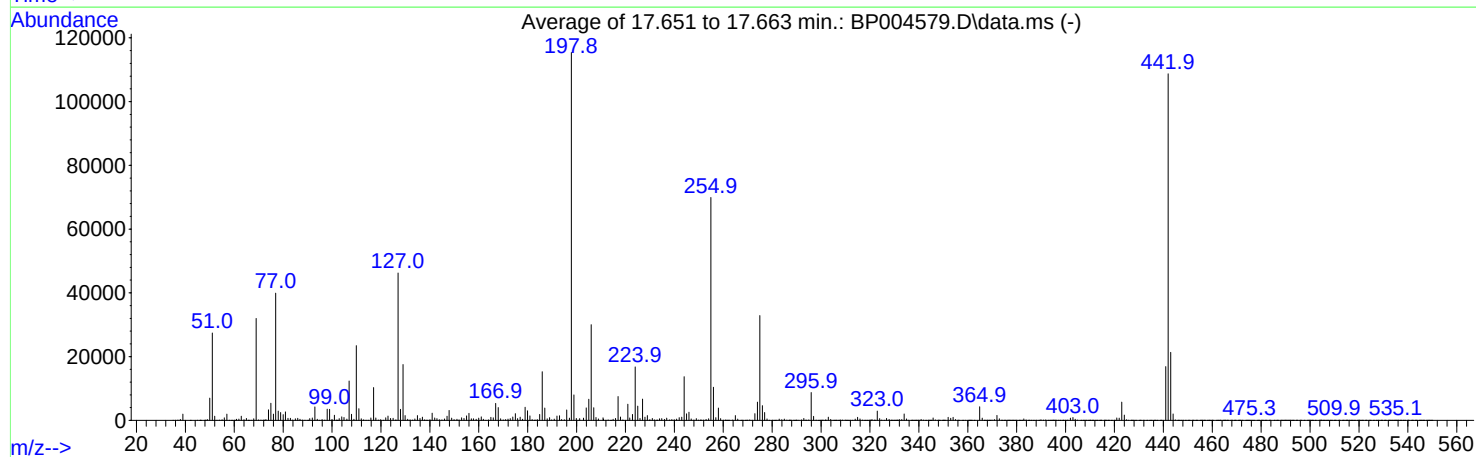


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011521\
 Data File : BP004579.D
 Acq On : 15 Jan 2021 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP011221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 12 15:19:32 2021

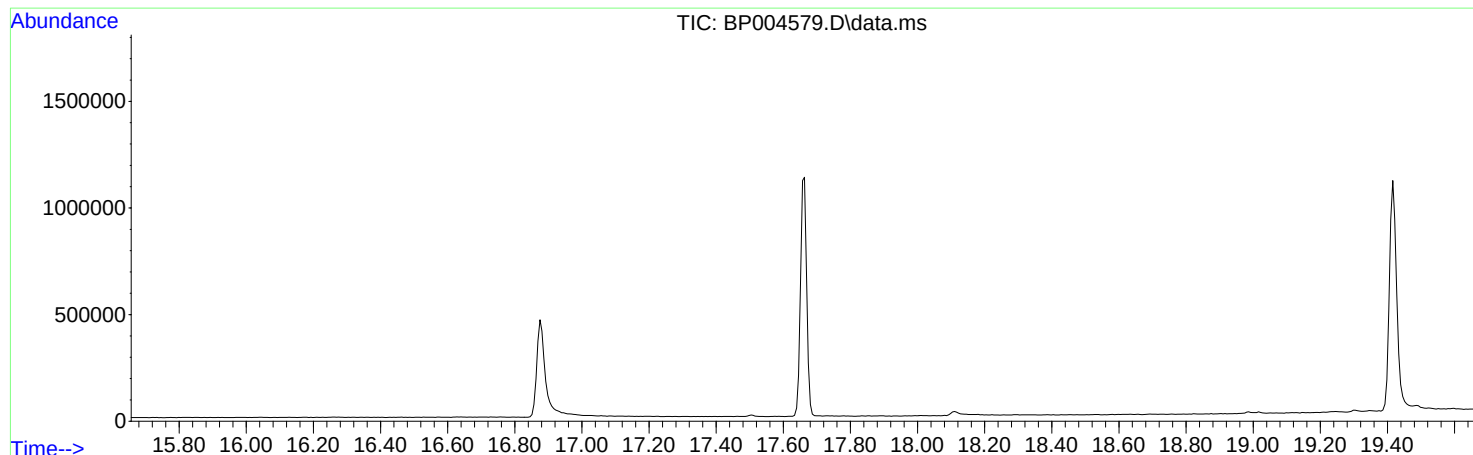

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	27413	PASS
68	69	0.00	2	1.5	488	PASS
69	198	0.00	100	27.7	32000	PASS
70	69	0.00	2	0.4	143	PASS
127	198	10	80	40.0	46217	PASS
197	198	0.00	2	0.6	685	PASS
198	198	100	100	100.0	115409	PASS
199	198	5	9	6.9	7965	PASS
275	198	10	60	28.5	32856	PASS
365	198	1	100	3.7	4289	PASS
441	198	0.01	100	14.6	16860	PASS
442	442	100	100	100.0	108731	PASS
443	442	15	24	19.6	21340	PASS