

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
 Data File : BP019376.D
 Acq On : 15 Jan 2024 17:50
 Operator : MA/JU
 Sample : P1130-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX0

Quant Time: Jan 15 23:51:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 03:05:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	112744	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.569	136	463094	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.416	164	325019	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.175	188	806048	20.000	ng/u1	-0.01
79) Chrysene-d12	21.280	240	775634	20.000	ng/u1	0.00
88) Perylene-d12	23.633	264	775873	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	12334	4.137	ng/uL	0.00
4) Pyridine-d5	3.640	84	90269	10.470	ng/u1	0.00
7) Phenol-d5	6.963	99	70091	6.504	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.116	67	243319	37.751	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.311	132	209357	28.283	ng/u1	0.00
15) 4-Methylphenol-d8	8.499	113	143527	16.789	ng/u1	-0.02
21) Nitrobenzene-d5	8.940	128	150146	38.539	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.657	143	167065	36.906	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.204	165	312484	34.168	ng/u1	0.00
31) 4-Chloroaniline-d4	10.722	131	268329	23.227	ng/u1	0.00
46) Dimethylphthalate-d6	13.840	166	1133313	39.468	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1187026	38.564	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.675	143	26885	6.097	ng/u1	0.00
60) Fluorene-d10	15.416	176	980970	41.727	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	214520	36.048	ng/u1	0.00
73) Anthracene-d10	17.275	188	1667712	41.484	ng/u1	-0.01
81) Pyrene-d10	19.522	212	2086748	41.259	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.480	264	1784470	42.298	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.246	88	133772	43.315	ng/uL	95
10) Bis(2-Chloroethyl)ether	7.205	93	9399	1.079	ng/u1#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019376.D
Acq On : 15 Jan 2024 17:50
Operator : MA/JU
Sample : P1130-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX0

Quant Time: Jan 15 23:51:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 09 03:05:24 2024
Response via : Initial Calibration

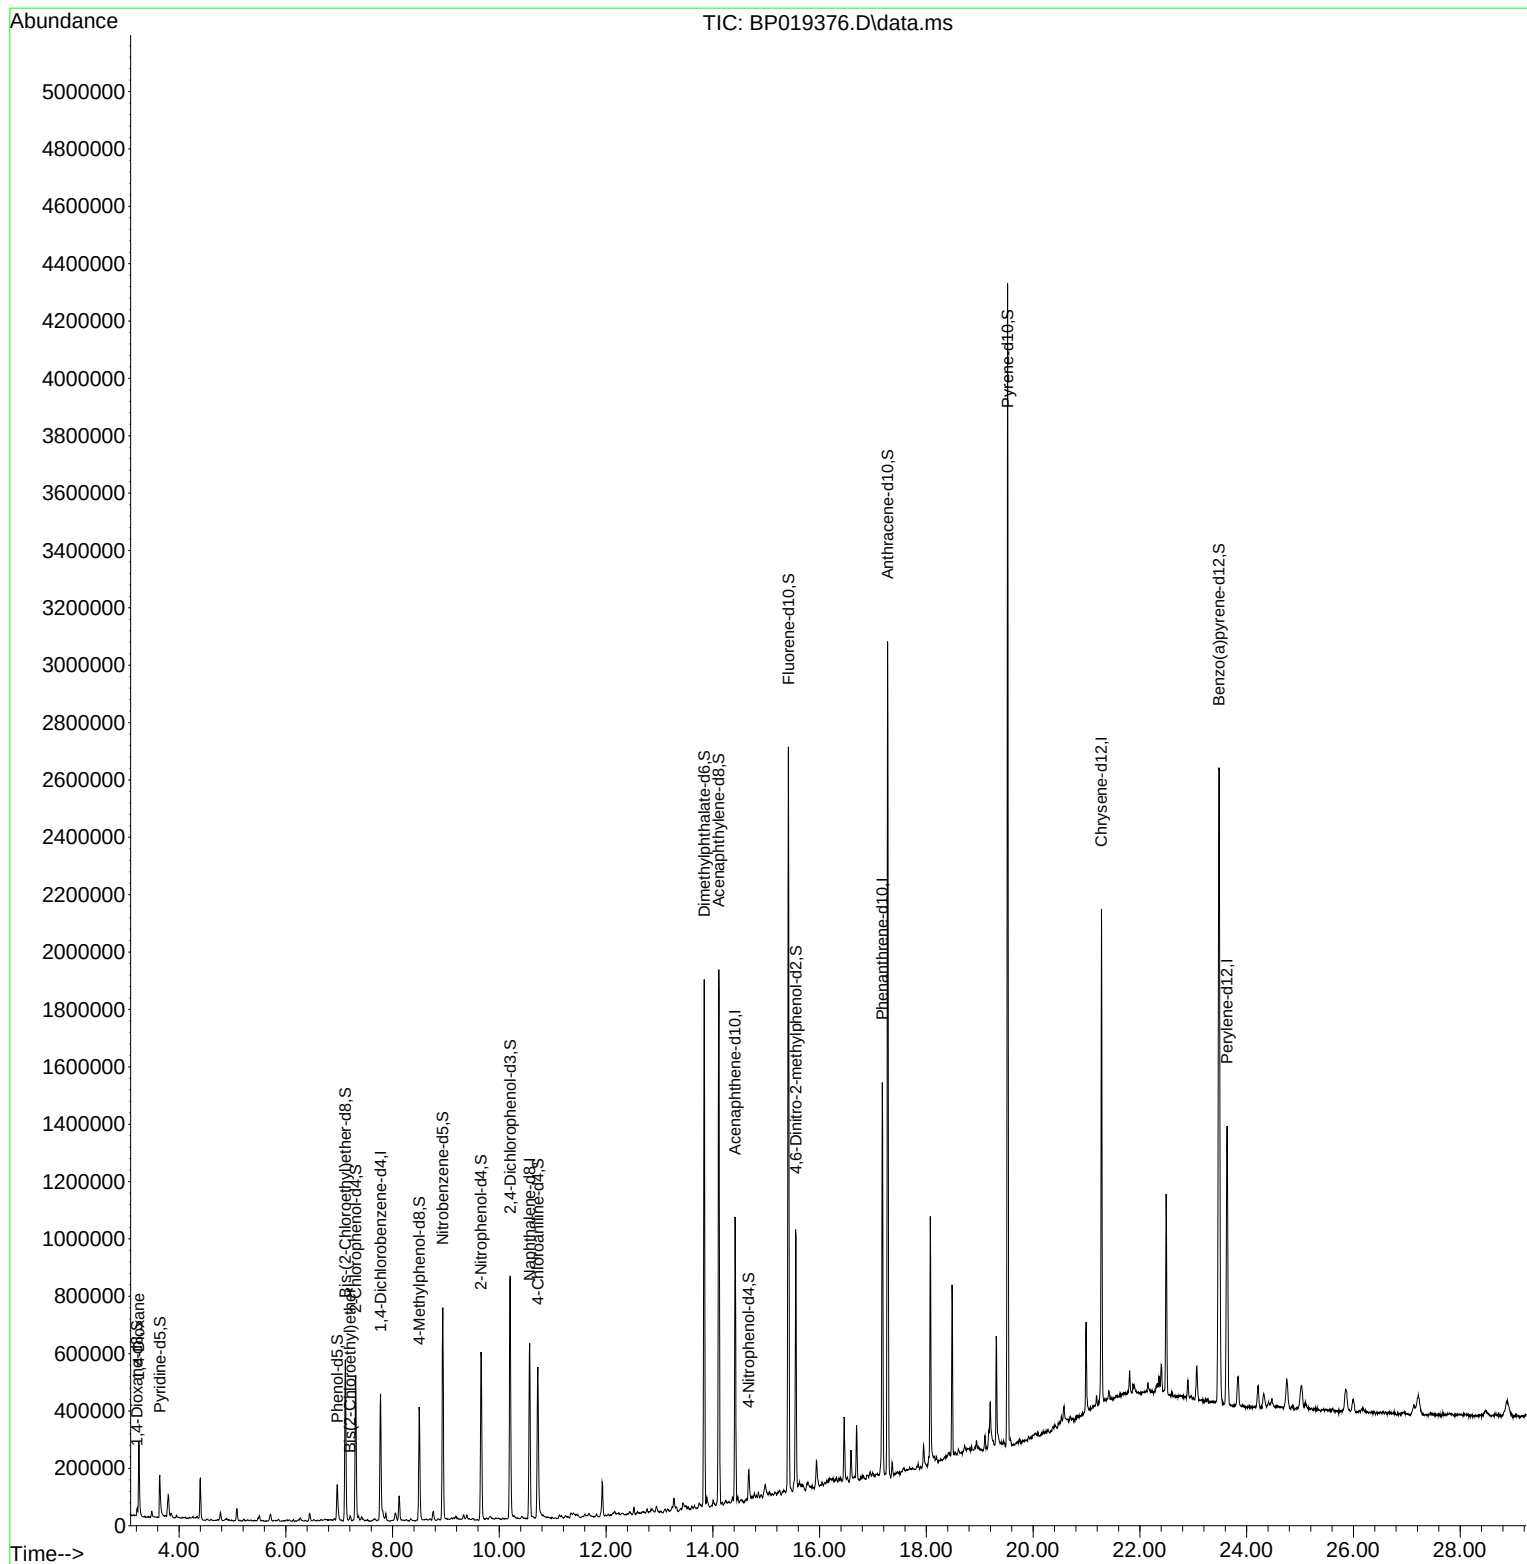




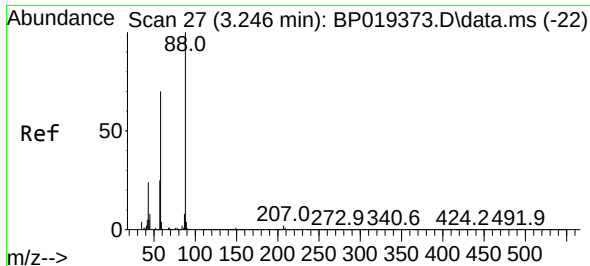


#2
 1,4-Dioxane
 Concen: 43.315 ng/uL
 RT: 3.246 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP019376.D
 Acq: 15 Jan 2024 17:50

Instrument :
 BNA_P
 ClientSampleId :
 COAX0

Tgt Ion: 88 Resp: 133772

Ion	Ratio	Lower	Upper
88	100		
43	28.3	22.0	33.0
58	73.2	54.6	82.0

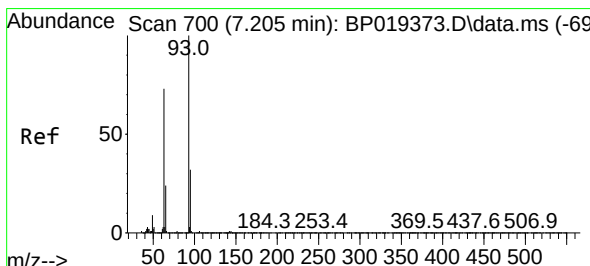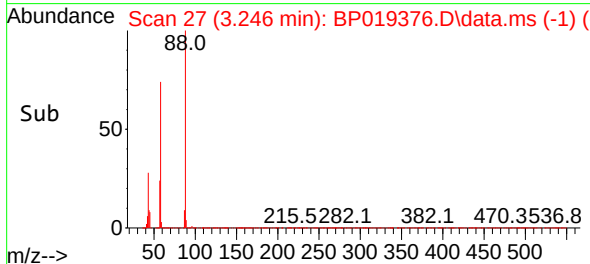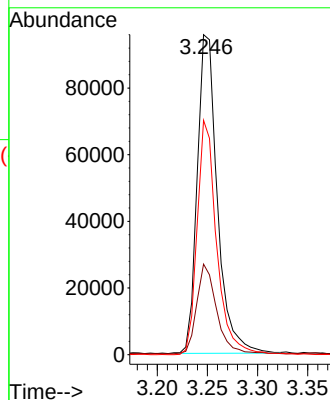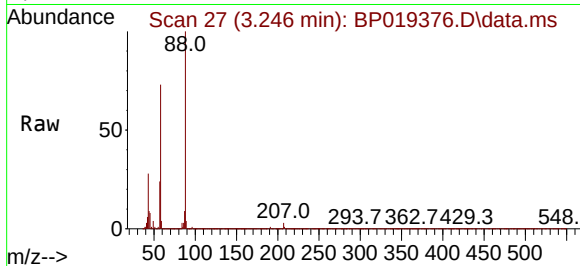

#10
 Bis(2-Chloroethyl)ether
 Concen: 1.079 ng/uL
 RT: 7.205 min Scan# 700
 Delta R.T. -0.012 min
 Lab File: BP019376.D
 Acq: 15 Jan 2024 17:50

Tgt Ion: 93 Resp: 9399

Ion	Ratio	Lower	Upper
93	100		
63	57.5	60.7	91.1
95	26.8	26.2	39.2

