

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
 Data File : BP019366.D
 Acq On : 15 Jan 2024 10:43
 Operator : MA/JU
 Sample : PB158426BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rBV	28755	38399	1.11%	0.116%
2	3.634	89	93	110	rBV	392897	632945	18.30%	1.911%
3	3.958	144	148	152	rVB5	5637	7710	0.22%	0.023%
4	6.963	652	659	669	rBV	479008	768138	22.21%	2.319%
5	7.116	678	685	693	rBV	376123	583685	16.88%	1.762%
6	7.310	711	718	731	rBV	464895	741580	21.45%	2.239%
7	7.775	790	797	809	rBV	422439	666748	19.28%	2.013%
8	8.498	914	920	931	rBV	578644	959474	27.75%	2.897%
9	8.940	988	995	1010	rBV	475961	799430	23.12%	2.414%
10	9.663	1111	1118	1128	rBV	413546	681418	19.71%	2.057%
11	10.204	1202	1210	1227	rBV	588081	1047649	30.30%	3.163%
12	10.569	1264	1272	1280	rBV	571921	952252	27.54%	2.875%
13	10.722	1290	1298	1318	rBV	550486	1026963	29.70%	3.101%
14	12.175	1538	1545	1554	rBV6	7474	16986	0.49%	0.051%
15	13.322	1736	1740	1747	rVB9	4248	7890	0.23%	0.024%
16	13.686	1798	1802	1807	rBV7	2475	4050	0.12%	0.012%
17	13.839	1821	1828	1840	rBV	1149314	1620504	46.86%	4.892%
18	14.110	1867	1874	1884	rBV	1246583	1816411	52.53%	5.484%
19	14.416	1918	1926	1934	rBV	917371	1375811	39.79%	4.154%
20	14.657	1961	1967	1987	rBV	389377	736420	21.30%	2.223%
21	15.416	2087	2096	2109	rBV	1736367	2394400	69.24%	7.229%
22	15.557	2113	2120	2133	rBV	523299	756298	21.87%	2.283%
23	15.657	2133	2137	2141	rVB4	8564	12620	0.36%	0.038%
24	15.827	2161	2166	2170	rBV8	2243	4546	0.13%	0.014%
25	16.198	2225	2229	2238	rVB8	5975	9604	0.28%	0.029%
26	16.857	2337	2341	2346	rVB7	3970	7013	0.20%	0.021%
27	17.174	2389	2395	2405	rBV	1294207	1861386	53.83%	5.620%
28	17.274	2405	2412	2427	rVV2	1891336	2709222	78.35%	8.179%
29	18.074	2546	2548	2552	rBV5	4056	4816	0.14%	0.015%
30	19.098	2717	2722	2727	rBV4	27874	41647	1.20%	0.126%
31	19.168	2730	2734	2740	rBV	24632	37338	1.08%	0.113%
32	19.521	2788	2794	2803	rBV	2712822	3458055	100.00%	10.440%
33	21.280	3088	3093	3100	rVB	1749021	2109496	61.00%	6.369%
34	23.480	3460	3467	3481	rVB	1702809	3231759	93.46%	9.757%
35	23.633	3486	3493	3504	rVB	1003073	1999677	57.83%	6.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019366.D
Acq On : 15 Jan 2024 10:43
Operator : MA/JU
Sample : PB158426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 33122340

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019366.D
Acq On : 15 Jan 2024 10:43
Operator : MA/JU
Sample : PB158426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

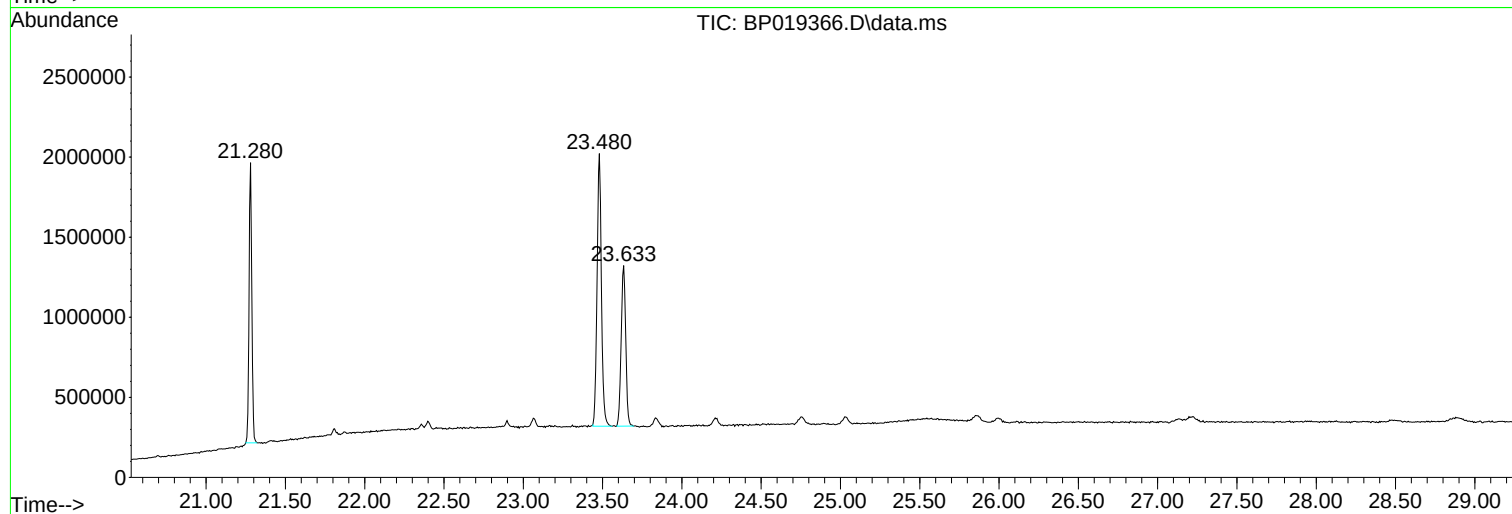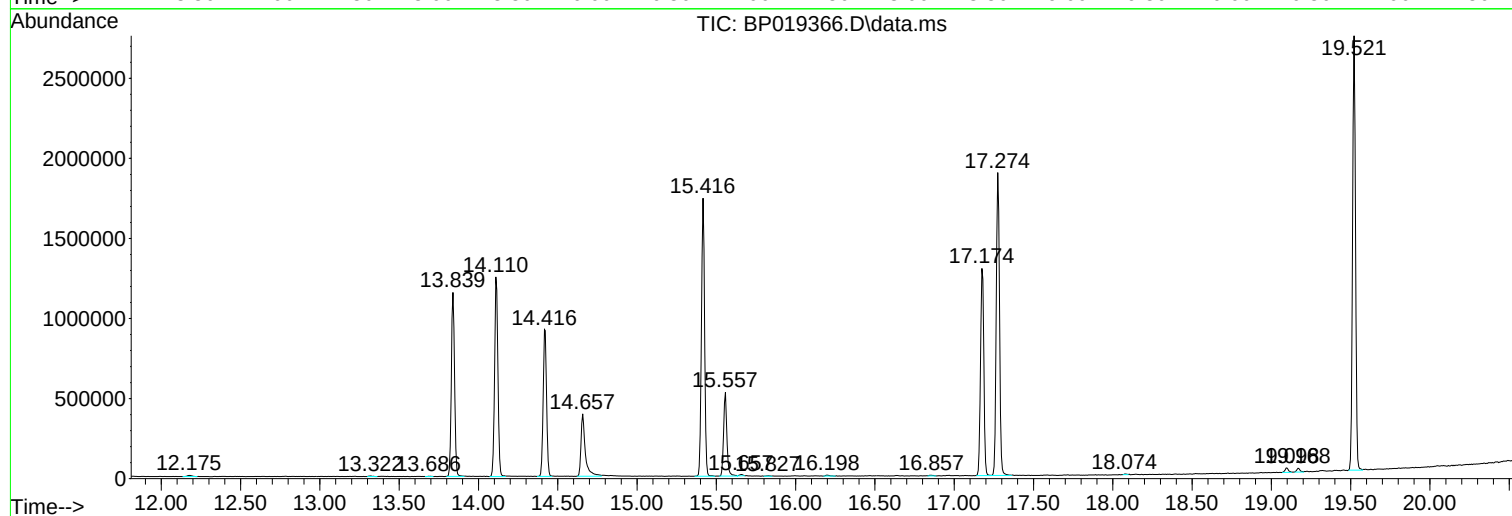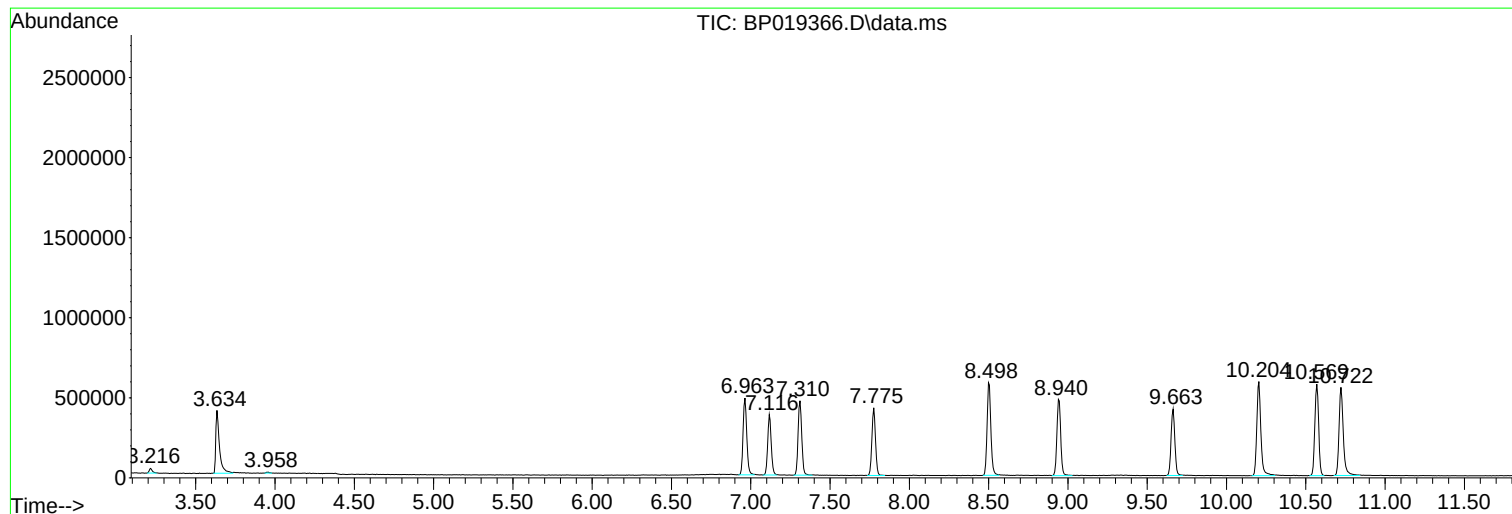

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019366.D
Acq On : 15 Jan 2024 10:43
Operator : MA/JU
Sample : PB158426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019366.D
Acq On : 15 Jan 2024 10:43
Operator : MA/JU
Sample : PB158426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc