

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
 Data File : BP019367.D
 Acq On : 15 Jan 2024 11:17
 Operator : MA/JU
 Sample : P1130-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	28	rVB	22969	31377	0.69%	0.086%
2	3.640	90	94	108	rBV	158837	270218	5.94%	0.737%
3	3.952	144	147	151	rVB2	7943	10761	0.24%	0.029%
4	4.881	299	305	311	rVB10	2474	5832	0.13%	0.016%
5	6.963	654	659	669	rBV	101623	175550	3.86%	0.479%
6	7.116	678	685	695	rBV	457858	709520	15.59%	1.935%
7	7.310	711	718	730	rBV	415140	678833	14.92%	1.852%
8	7.775	789	797	807	rBV	452288	704378	15.48%	1.921%
9	8.499	914	920	933	rBV	322044	551585	12.12%	1.505%
10	8.940	988	995	1006	rBV	590595	963308	21.17%	2.628%
11	9.328	1058	1061	1068	rVB8	4153	9019	0.20%	0.025%
12	9.663	1110	1118	1130	rBV	477763	803427	17.66%	2.191%
13	10.204	1202	1210	1227	rBV	642312	1172756	25.77%	3.199%
14	10.569	1263	1272	1281	rBV	616367	1012049	22.24%	2.761%
15	10.722	1289	1298	1316	rBV	600185	1097044	24.11%	2.992%
16	12.175	1538	1545	1550	rBV3	9666	18526	0.41%	0.051%
17	13.393	1745	1752	1757	rBV3	3505	5969	0.13%	0.016%
18	13.840	1821	1828	1841	rBV	1418660	1931242	42.44%	5.268%
19	14.110	1865	1874	1888	rBV	1462295	2152598	47.31%	5.872%
20	14.422	1919	1927	1935	rBV	941960	1435930	31.56%	3.917%
21	14.669	1964	1969	1979	rBV	58942	140486	3.09%	0.383%
22	14.775	1985	1987	1993	rVB7	3763	5784	0.13%	0.016%
23	15.416	2086	2096	2108	rBV	2016795	2852039	62.68%	7.779%
24	15.557	2113	2120	2133	rBV	727131	1048239	23.04%	2.859%
25	15.657	2133	2137	2144	rVB7	9614	19354	0.43%	0.053%
26	16.204	2225	2230	2235	rBV8	8307	14121	0.31%	0.039%
27	16.586	2288	2295	2300	rBV10	6345	14865	0.33%	0.041%
28	16.769	2320	2326	2331	rVB4	11615	19625	0.43%	0.054%
29	16.939	2352	2355	2357	rBV4	3224	4769	0.10%	0.013%
30	17.175	2389	2395	2402	rBV	1373571	1889868	41.53%	5.155%
31	17.275	2405	2412	2425	rBV	2500834	3470197	76.27%	9.466%
32	17.575	2461	2463	2468	rVB6	4775	6074	0.13%	0.017%
33	17.945	2524	2526	2530	rBV4	5352	6637	0.15%	0.018%
34	18.069	2543	2547	2551	rBV	68195	88437	1.94%	0.241%
35	18.480	2613	2617	2622	rBV	69414	80640	1.77%	0.220%
36	19.098	2718	2722	2726	rBV2	38167	53823	1.18%	0.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019367.D
Acq On : 15 Jan 2024 11:17
Operator : MA/JU
Sample : P1130-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	19.169	2730	2734	2738	rBV	34414	52264	1.15%	0.143%
38	19.310	2754	2758	2762	rBV3	43036	57962	1.27%	0.158%
39	19.522	2788	2794	2800	rBV	3583189	4550176	100.00%	12.411%
40	21.280	3088	3093	3100	rBV	1740410	2146327	47.17%	5.854%
41	22.492	3296	3299	3304	rVB	103255	140912	3.10%	0.384%
42	23.480	3460	3467	3479	rVB	2210242	4202929	92.37%	11.464%
43	23.633	3486	3493	3503	rVB	1056273	2055994	45.18%	5.608%




Sum of corrected areas: 36661444

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019367.D
Acq On : 15 Jan 2024 11:17
Operator : MA/JU
Sample : P1130-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

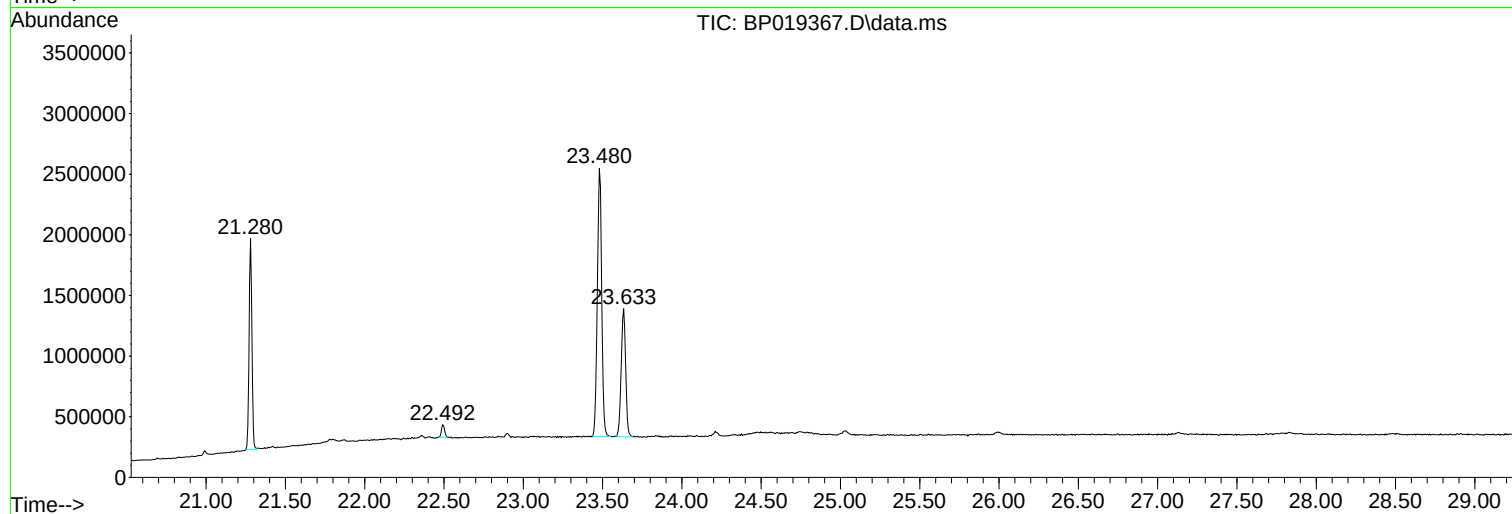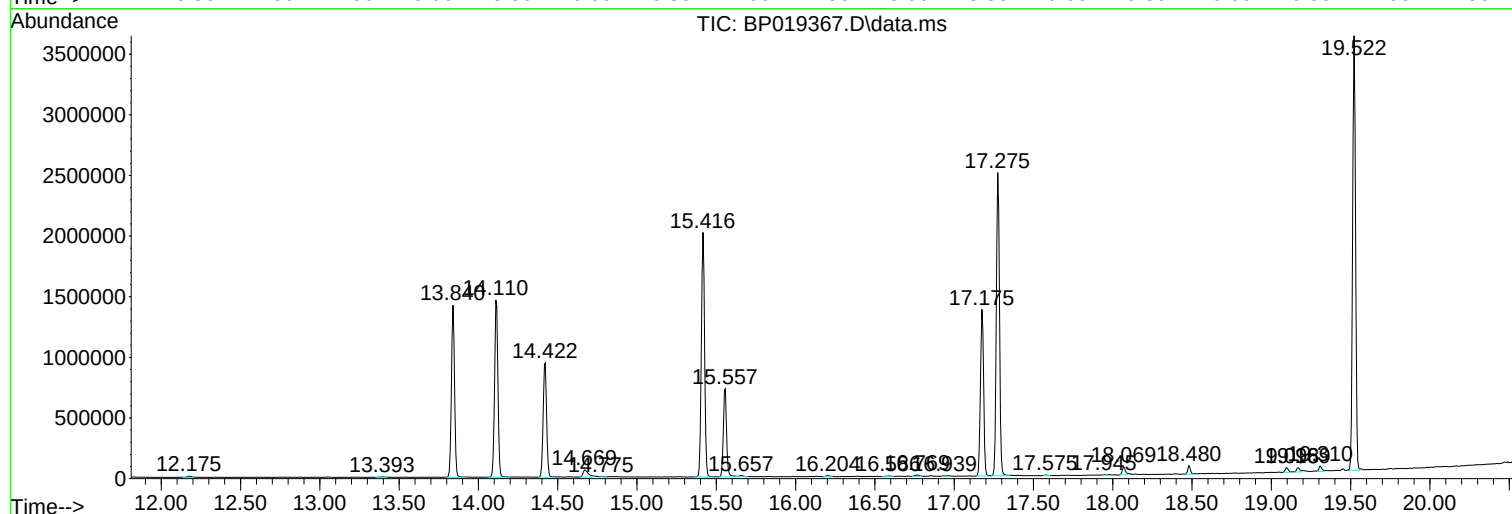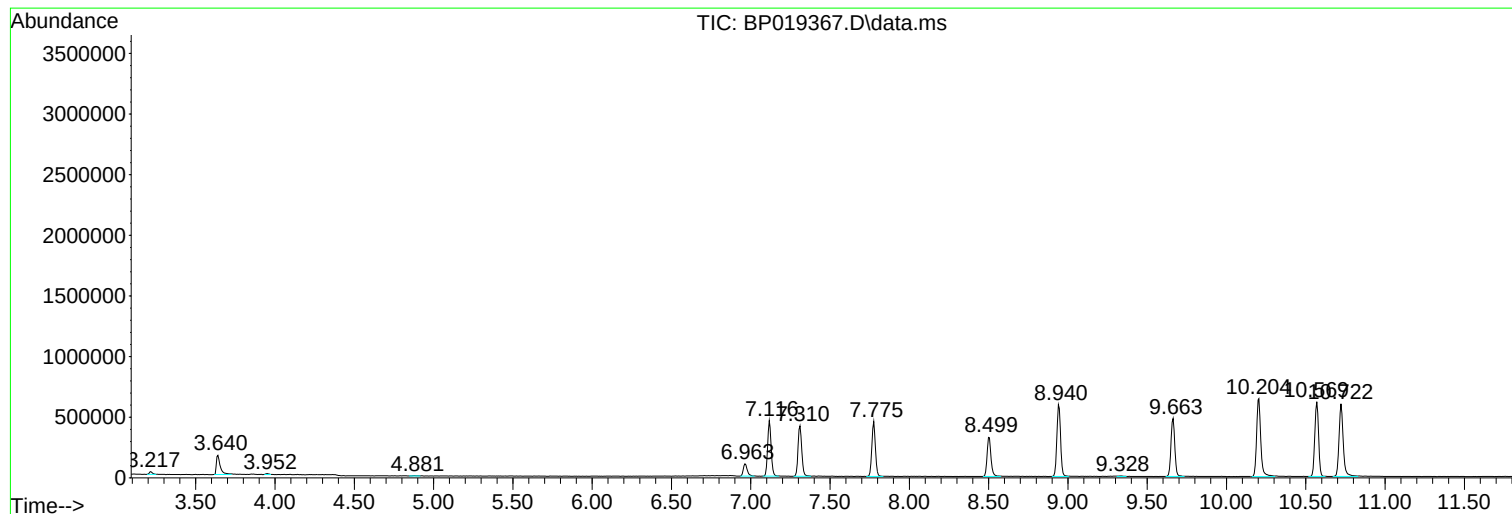

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019367.D
Acq On : 15 Jan 2024 11:17
Operator : MA/JU
Sample : P1130-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019367.D
Acq On : 15 Jan 2024 11:17
Operator : MA/JU
Sample : P1130-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc