

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
 Data File : BP019370.D
 Acq On : 15 Jan 2024 12:59
 Operator : MA/JU
 Sample : P1130-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	28	rBV	25519	34466	0.68%	0.084%
2	3.640	91	94	110	rBV	130106	220908	4.39%	0.536%
3	3.858	128	131	134	rVB3	5368	6066	0.12%	0.015%
4	3.952	143	147	151	rBV	10800	14844	0.30%	0.036%
5	6.964	653	659	674	rVB	119553	211242	4.20%	0.512%
6	7.117	678	685	699	rBV	583150	902706	17.94%	2.189%
7	7.311	710	718	729	rBV	509408	815821	16.21%	1.979%
8	7.775	788	797	805	rBV	476722	734425	14.60%	1.781%
9	8.046	838	843	846	rBV7	3873	6257	0.12%	0.015%
10	8.499	913	920	934	rBV	374452	639057	12.70%	1.550%
11	8.611	934	939	946	rVB3	16067	28512	0.57%	0.069%
12	8.940	988	995	1011	rBV	750714	1225546	24.36%	2.972%
13	9.075	1013	1018	1022	rBV8	6580	12969	0.26%	0.031%
14	9.334	1059	1062	1067	rVB7	4361	6515	0.13%	0.016%
15	9.663	1110	1118	1128	rBV	559898	926009	18.40%	2.246%
16	10.199	1200	1209	1231	rBV	787087	1421578	28.25%	3.448%
17	10.569	1264	1272	1282	rVB	637679	1046575	20.80%	2.538%
18	10.722	1290	1298	1315	rBV	752276	1343657	26.70%	3.259%
19	11.128	1362	1367	1372	rBV5	4698	9106	0.18%	0.022%
20	11.193	1374	1378	1383	rVB5	4850	8347	0.17%	0.020%
21	11.581	1439	1444	1452	rBV5	5845	10437	0.21%	0.025%
22	12.169	1538	1544	1553	rVB	14474	27424	0.55%	0.067%
23	12.310	1560	1568	1573	rBV8	5899	12721	0.25%	0.031%
24	12.675	1627	1630	1635	rBV6	4423	8073	0.16%	0.020%
25	12.857	1653	1661	1668	rBV	31890	66058	1.31%	0.160%
26	13.322	1734	1740	1747	rBV3	17592	30757	0.61%	0.075%
27	13.393	1747	1752	1754	rVV5	3510	5865	0.12%	0.014%
28	13.434	1754	1759	1765	rVB10	5732	10713	0.21%	0.026%
29	13.751	1807	1813	1817	rBV9	4126	8771	0.17%	0.021%
30	13.840	1820	1828	1840	rBV	1811559	2451225	48.72%	5.945%
31	14.110	1865	1874	1888	rBV	1861368	2748328	54.62%	6.666%
32	14.422	1920	1927	1939	rBV	1017074	1505785	29.93%	3.652%
33	14.669	1963	1969	1985	rBV	52211	140611	2.79%	0.341%
34	14.875	1999	2004	2008	rVB8	5507	8764	0.17%	0.021%
35	15.416	2087	2096	2104	rBV	2588794	3607919	71.70%	8.751%
36	15.557	2111	2120	2128	rBV	666904	938549	18.65%	2.276%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
 Data File : BP019370.D
 Acq On : 15 Jan 2024 12:59
 Operator : MA/JU
 Sample : P1130-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	15.628	2128	2132	2148	rVB2	51645	99053	1.97%	0.240%
38	16.204	2224	2230	2235	rVB3	9972	15924	0.32%	0.039%
39	16.728	2314	2319	2323	rBV7	6254	10628	0.21%	0.026%
40	16.851	2336	2340	2344	rBV6	5440	8648	0.17%	0.021%
41	16.975	2355	2361	2363	rBV6	4259	7896	0.16%	0.019%
42	17.175	2388	2395	2405	rBV	1441928	1959821	38.95%	4.753%
43	17.275	2405	2412	2426	rVV2	2899000	4110381	81.69%	9.969%
44	17.392	2429	2432	2438	rVB8	5122	8209	0.16%	0.020%
45	17.910	2516	2520	2527	rVB7	13533	20849	0.41%	0.051%
46	18.069	2543	2547	2555	rBV7	22944	34630	0.69%	0.084%
47	19.098	2718	2722	2729	rVB2	38983	58113	1.15%	0.141%
48	19.169	2729	2734	2740	rBV	40222	59666	1.19%	0.145%
49	19.216	2740	2742	2745	rVB4	5997	5720	0.11%	0.014%
50	19.310	2755	2758	2762	rBV6	8802	11353	0.23%	0.028%
51	19.451	2779	2782	2787	rBV7	10235	14341	0.29%	0.035%
52	19.522	2788	2794	2807	rBV	3886928	5031692	100.00%	12.204%
53	21.280	3088	3093	3101	rBV	1698784	2137694	42.48%	5.185%
54	23.480	3460	3467	3480	rVB	2285377	4449881	88.44%	10.793%
55	23.633	3486	3493	3506	rVB	1012595	1989895	39.55%	4.826%




Sum of corrected areas: 41231000

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019370.D
Acq On : 15 Jan 2024 12:59
Operator : MA/JU
Sample : P1130-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

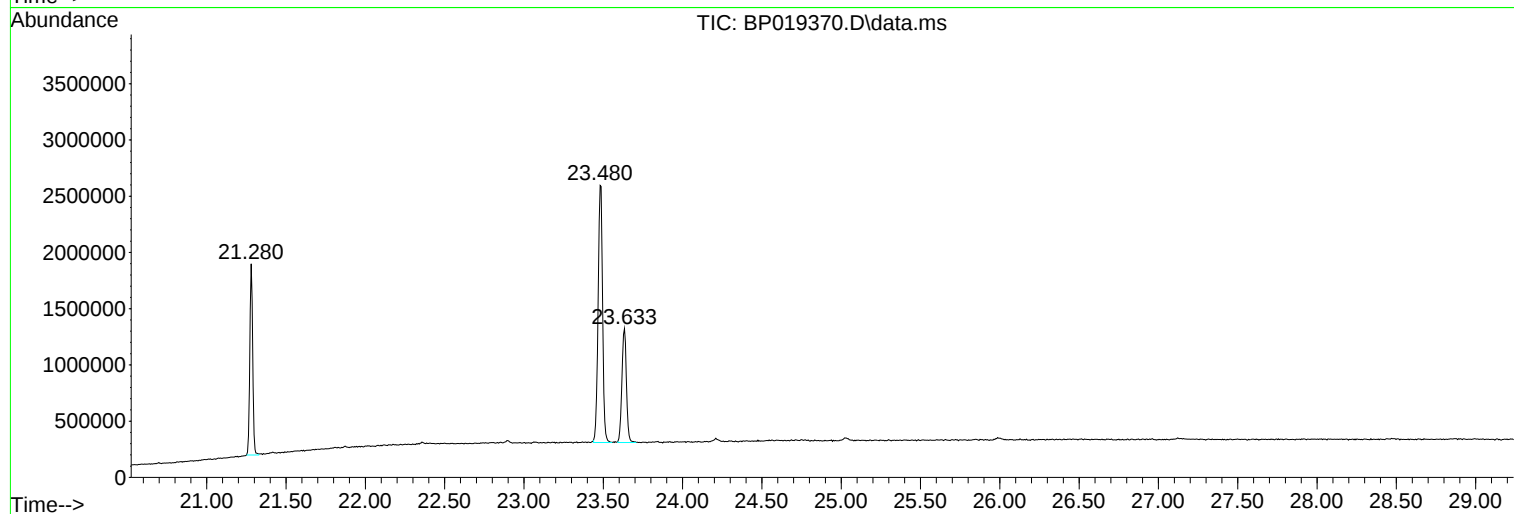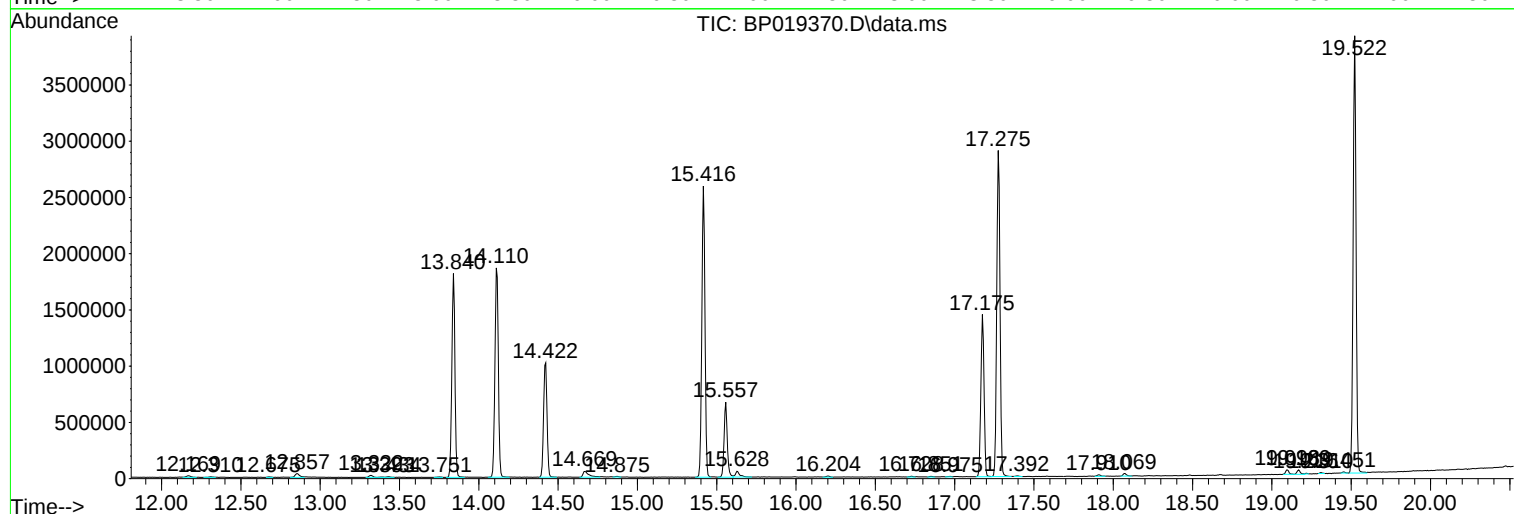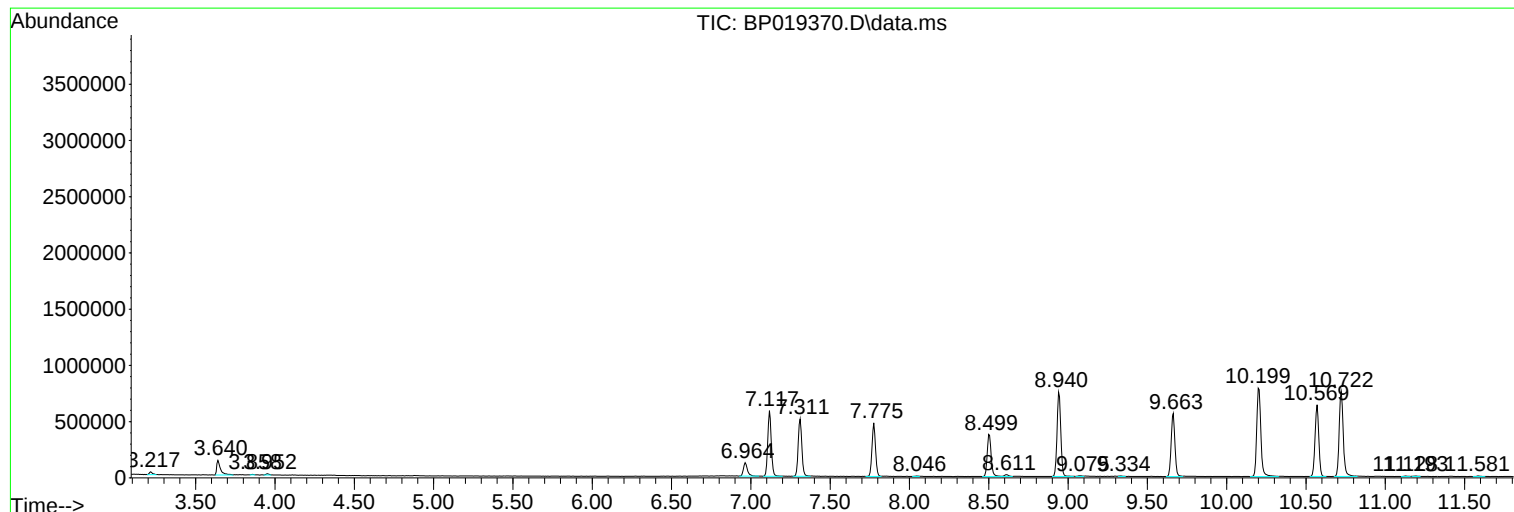

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019370.D
Acq On : 15 Jan 2024 12:59
Operator : MA/JU
Sample : P1130-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011524\
Data File : BP019370.D
Acq On : 15 Jan 2024 12:59
Operator : MA/JU
Sample : P1130-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
