
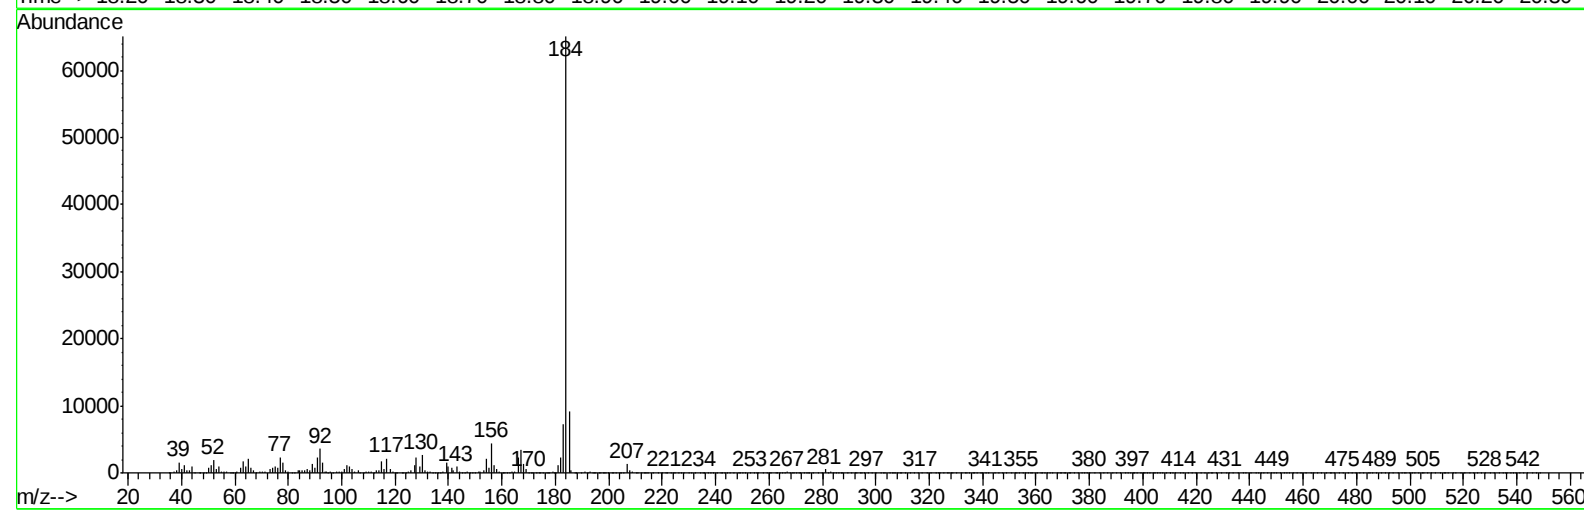


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP011620\
 Data File : BP001629.D
 Acq On : 16 Jan 2020 15:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 06:56:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 21:52:04 2020
 Response via : Initial Calibration

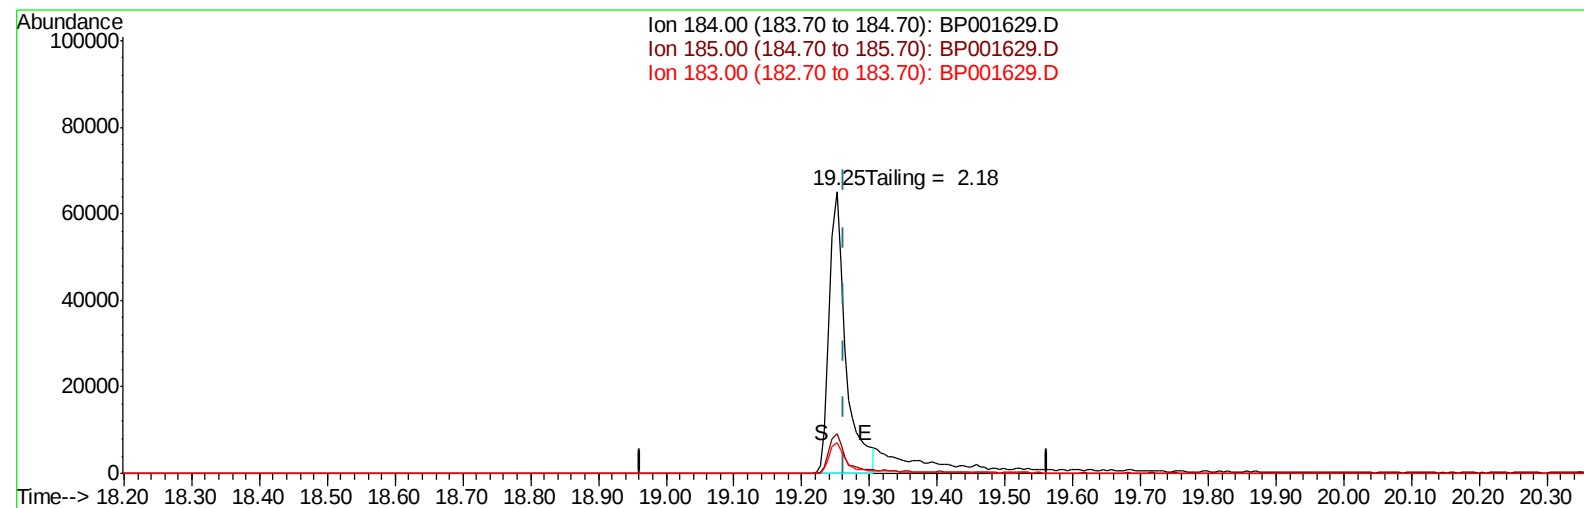

TIC: BP001629.D

(77) Benzidine



19.251min (-0.012) 40683.04ng

response 120762

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	14.08
183.00	11.70	11.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP011620\
Data File : BP001629.D
Acq On : 16 Jan 2020 15:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 06:56:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

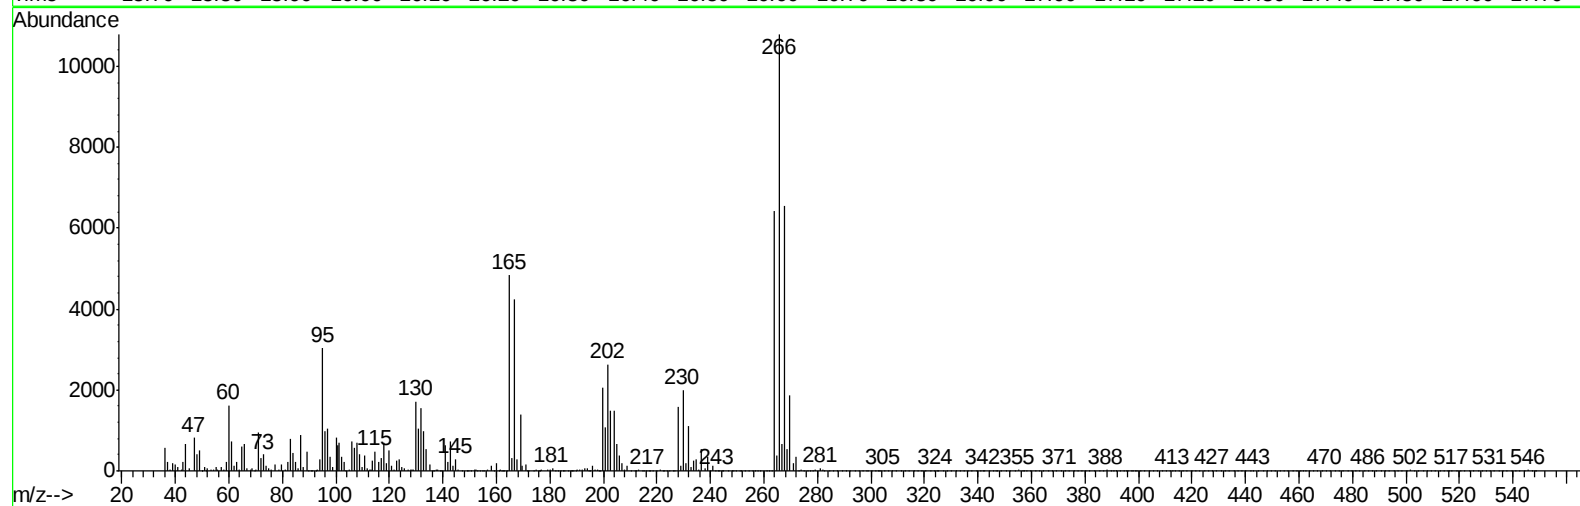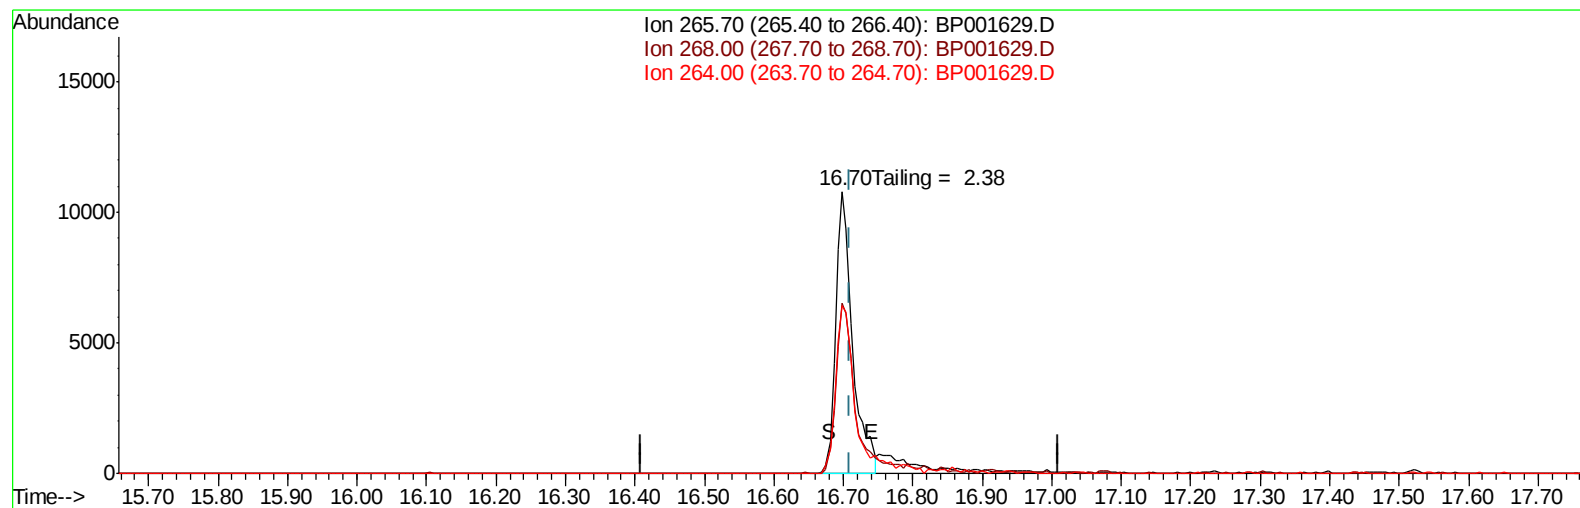

TIC: BP001629.D

(70) Pentachlorophenol (C)

16.698min (-0.012) 91648.95ng

response 18575

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	60.67
264.00	63.60	59.48
0.00	0.00	0.00