

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011620\
 Data File : BP001648.D
 Acq On : 17 Jan 2020 02:34
 Operator : JU
 Sample : L1111-07 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONCRETE-FLOOR

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.869	10	14	23	rBV5	14011	28830	3.13%	0.360%
2	2.946	23	27	40	rVB	95834	128745	14.00%	1.609%
3	4.798	337	342	349	rVB	139297	187988	20.44%	2.350%
4	5.263	415	421	435	rVB	318571	470572	51.17%	5.882%
5	6.834	681	688	702	rBV	348414	567692	61.73%	7.096%
6	6.940	702	706	713	rVB2	7704	13156	1.43%	0.164%
7	7.175	739	746	755	rBV	343119	542101	58.94%	6.776%
8	7.634	817	824	831	rBV	194745	303885	33.04%	3.798%
9	7.951	871	878	888	rVB	290674	448158	48.73%	5.602%
10	8.781	1012	1019	1030	rVB	208862	354400	38.53%	4.430%
11	10.410	1288	1296	1307	rBV	221720	376252	40.91%	4.703%
12	12.898	1712	1719	1732	rBV	499092	742395	80.72%	9.280%
13	13.745	1855	1863	1869	rBV	34751	51342	5.58%	0.642%
14	14.280	1948	1954	1963	rBV	325426	497048	54.04%	6.213%
15	15.116	2090	2096	2101	rBV6	5399	9345	1.02%	0.117%
16	15.786	2204	2210	2220	rBV	327490	491532	53.44%	6.144%
17	16.839	2386	2389	2396	rVB5	8869	11289	1.23%	0.141%
18	17.045	2418	2424	2435	rBV	394831	564470	61.38%	7.056%
19	19.627	2858	2863	2869	rBV	750610	919697	100.00%	11.496%
20	20.439	2999	3001	3005	rBV	22849	24372	2.65%	0.305%
21	20.892	3075	3078	3083	rVB2	65526	80405	8.74%	1.005%
22	21.151	3117	3122	3128	rBV	371358	493288	53.64%	6.166%
23	21.762	3223	3226	3229	rBV	48883	49359	5.37%	0.617%
24	22.227	3303	3305	3312	rVB	80014	92547	10.06%	1.157%
25	22.739	3390	3392	3400	rVB	73705	101375	11.02%	1.267%
26	23.380	3496	3501	3511	rVB	238603	449902	48.92%	5.624%


Sum of corrected areas: 8000145

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP011620\
Data File : BP001648.D
Acq On : 17 Jan 2020 02:34
Operator : JU
Sample : L1111-07 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONCRETE-FLOOR

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

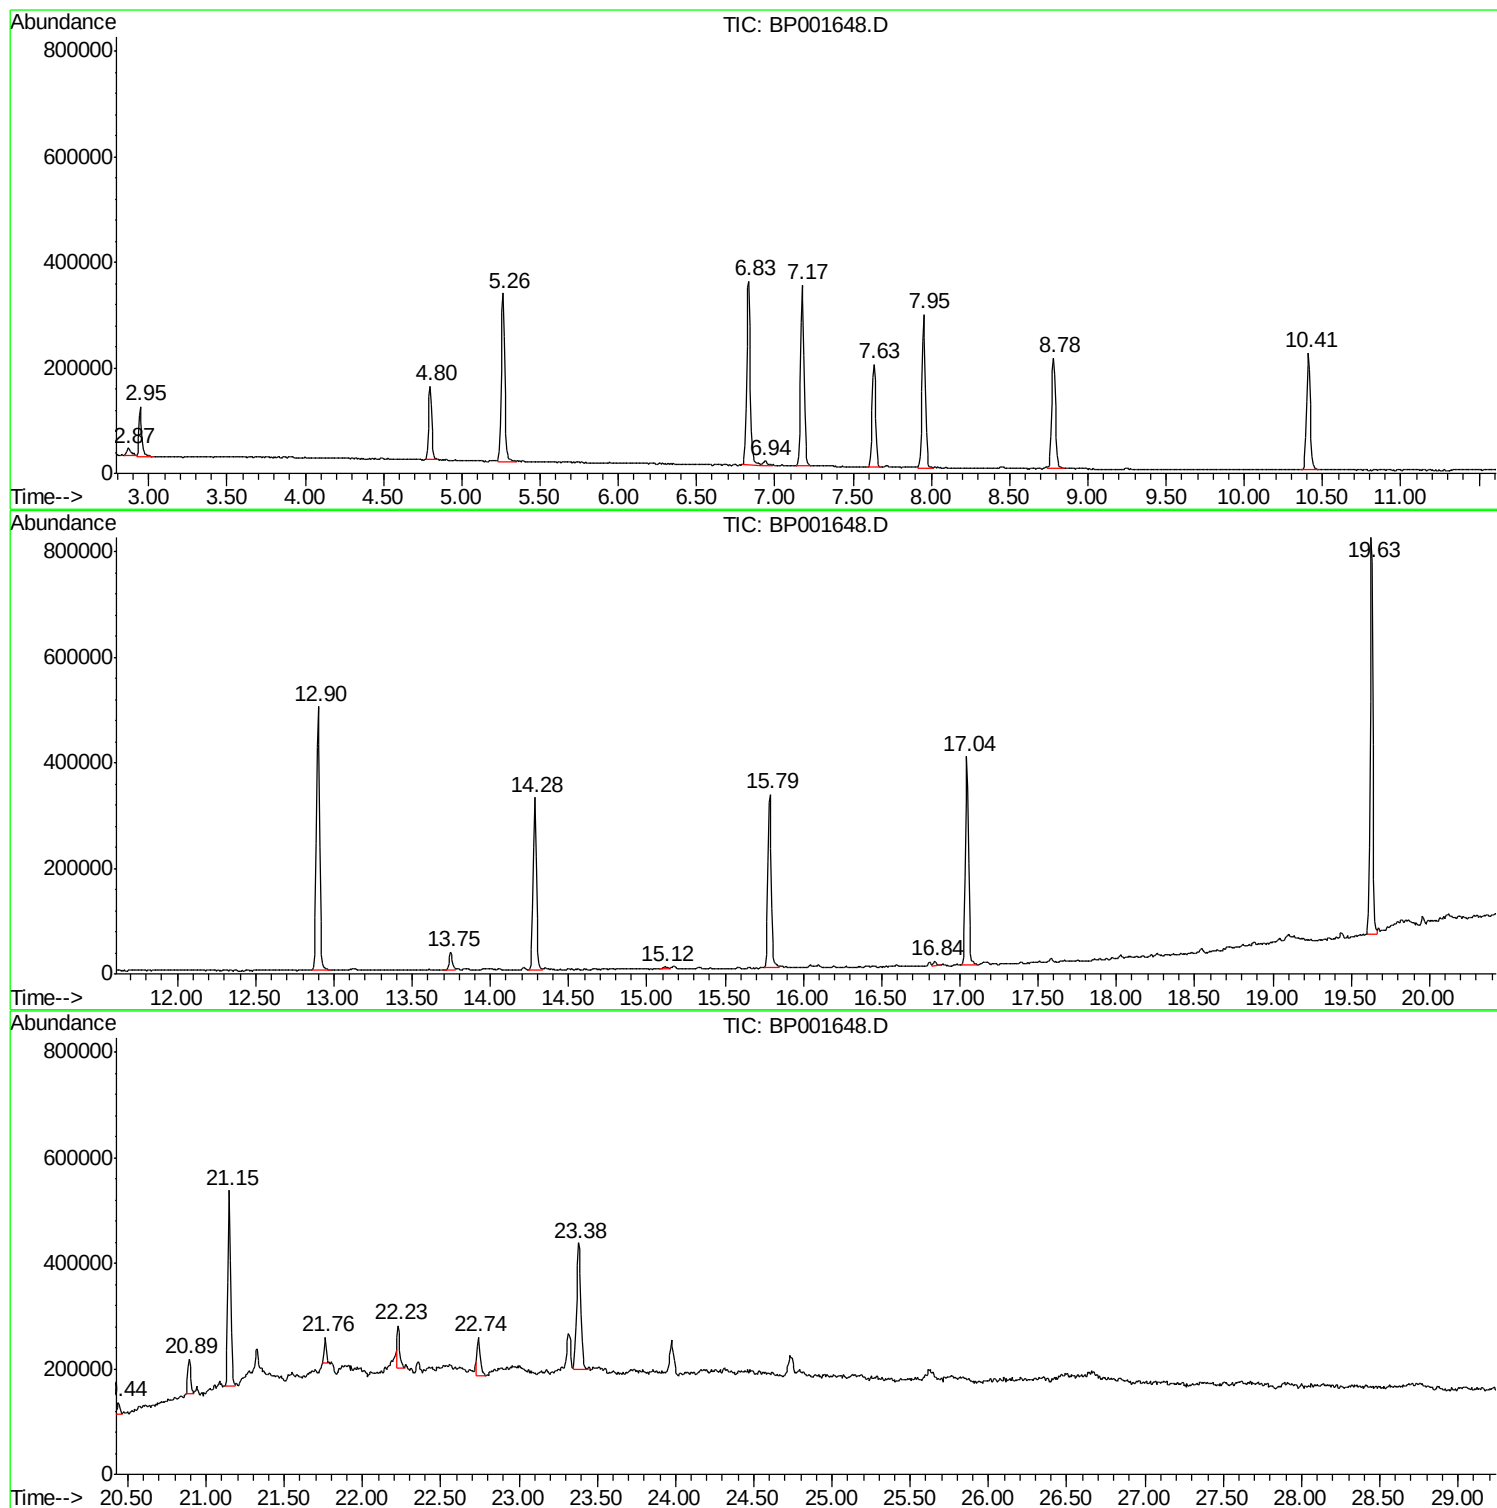

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011620\
Data_File : BP001648.D
Acq_On : 17 Jan 2020 02:344
Operator : JUJ
Sample : L1111-07.2XX
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
CONCRETE-FLOOR

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
