


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011620\
 Data File : BP001629.D
 Acq On : 16 Jan 2020 15:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 21:52:04 2020

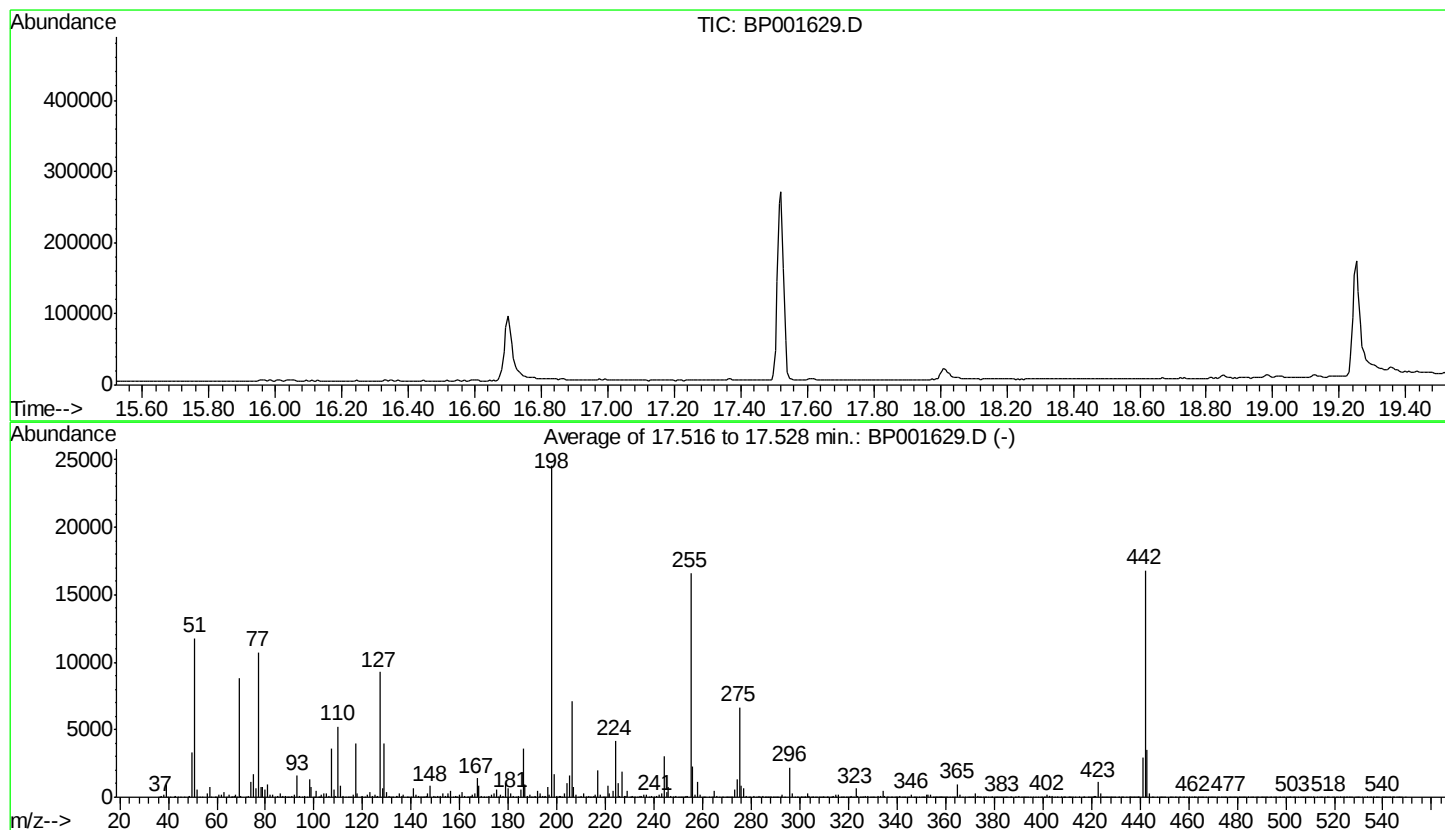

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	11798	PASS
68	69	0.00	2	2.0	178	PASS
69	198	0.00	100	35.9	8830	PASS
70	69	0.00	2	0.7	65	PASS
127	198	10	80	37.7	9257	PASS
197	198	0.00	2	0.7	177	PASS
198	198	100	100	100.0	24565	PASS
199	198	5	9	6.8	1669	PASS
275	198	10	60	27.0	6640	PASS
365	198	1	100	4.0	976	PASS
441	198	0.01	100	12.1	2970	PASS
442	198	50	100	68.4	16802	PASS
443	442	15	24	21.0	3534	PASS