

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
 Data File : BP013475.D
 Acq On : 16 Jan 2023 10:42
 Operator : CG/JU
 Sample : PB150192BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150192BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	301	307	317	rBV	4410768	6137660	15.88%	3.664%
2	5.464	380	387	397	rBV	10294356	14652695	37.92%	8.747%
3	7.075	652	661	675	rBV	9668093	15695895	40.62%	9.369%
4	7.905	794	802	811	rBV	1791753	2744696	7.10%	1.638%
5	9.075	993	1001	1021	rBV	5998643	9694559	25.09%	5.787%
6	10.716	1272	1280	1294	rVB	2351479	3963984	10.26%	2.366%
7	13.175	1690	1698	1713	rBV	15463754	23399140	60.56%	13.968%
8	14.551	1925	1932	1946	rBV	3880485	5742399	14.86%	3.428%
9	16.051	2179	2187	2208	rBV	14279857	20701067	53.58%	12.357%
10	17.310	2395	2401	2412	rBV	5110964	7461282	19.31%	4.454%
11	19.869	2830	2836	2841	rBV	29792656	38638767	100.00%	23.065%
12	21.404	3092	3097	3103	rBV	7002109	8879336	22.98%	5.300%
13	23.863	3509	3515	3528	rVB2	4879350	9813060	25.40%	5.858%




Sum of corrected areas: 167524540

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
Data File : BP013475.D
Acq On : 16 Jan 2023 10:42
Operator : CG/JU
Sample : PB150192BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150192BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

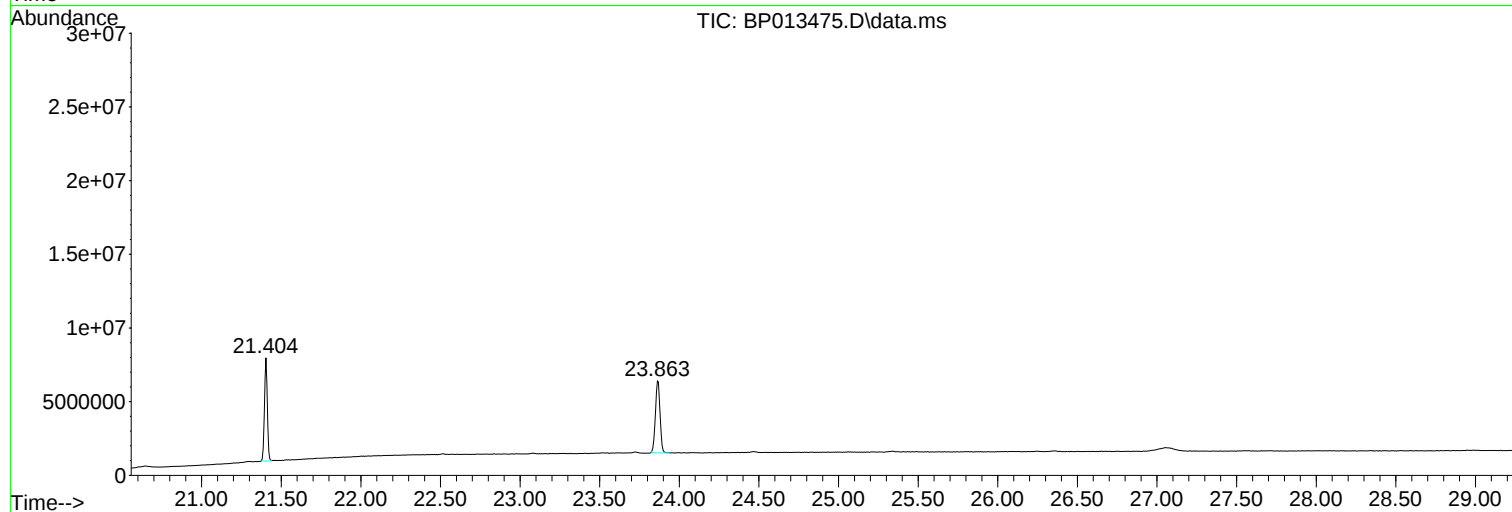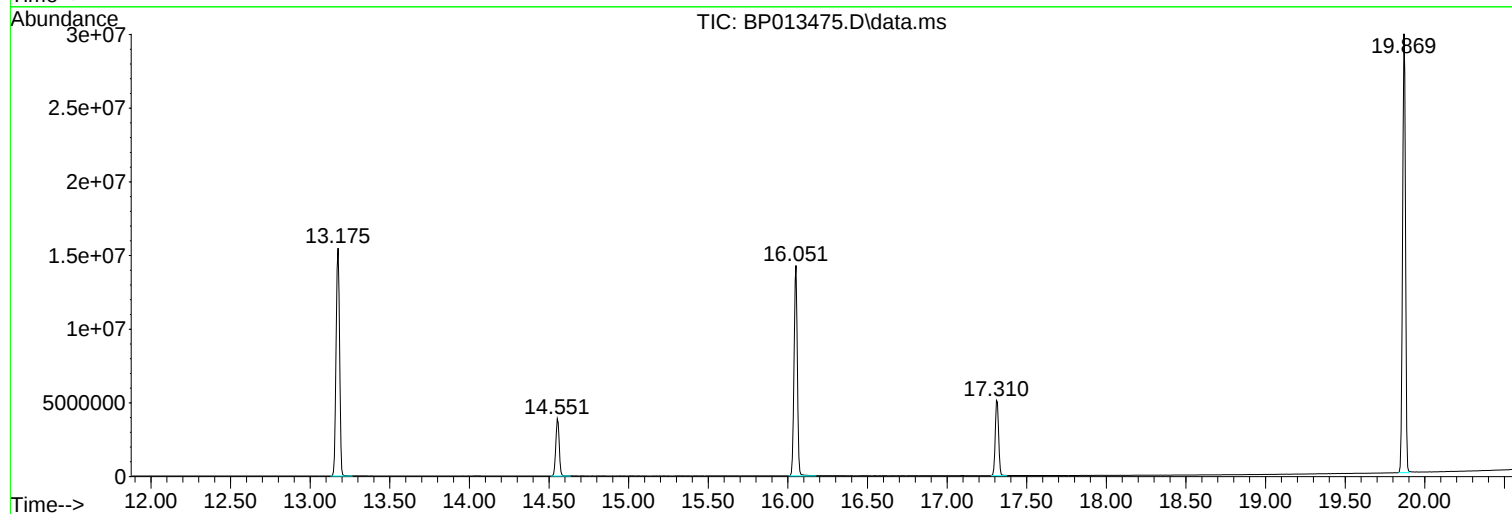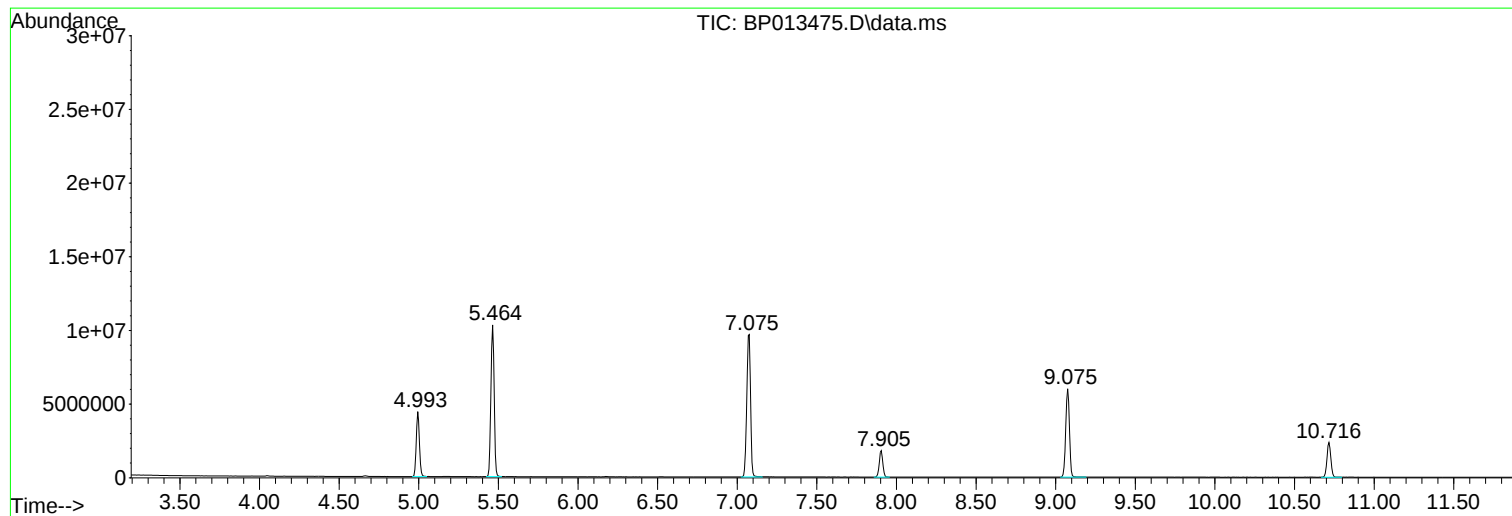

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
Data File : BP013475.D
Acq On : 16 Jan 2023 10:42
Operator : CG/JU
Sample : PB150192BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150192BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.993	44.72 ng	6137660	1,4-Dichlorobenzene-d4	7.905

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

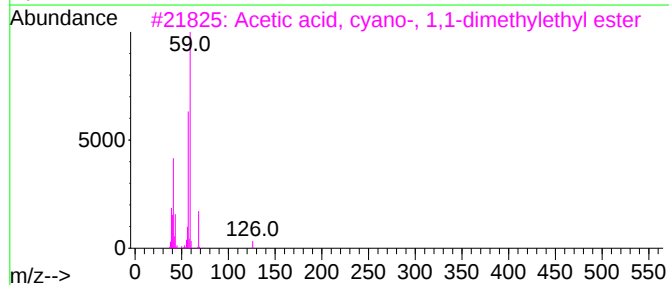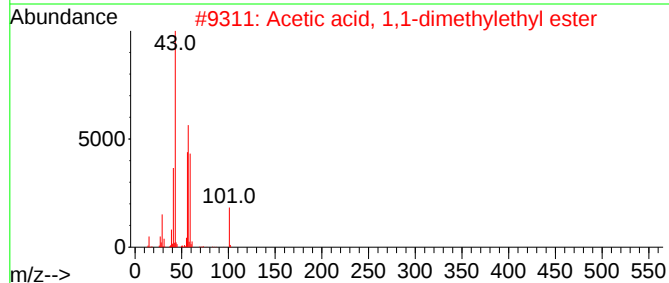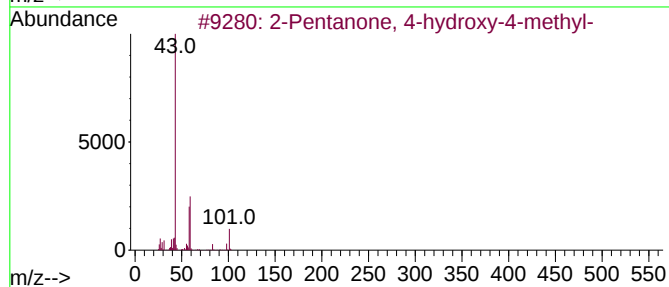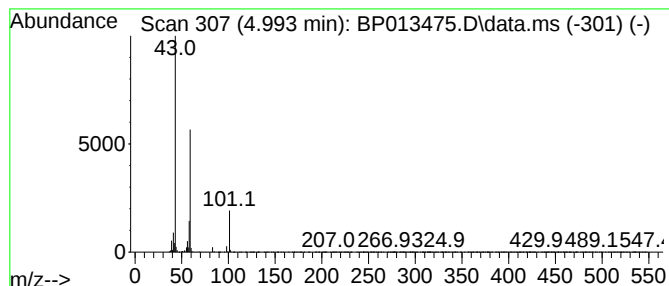

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
Data File : BP013475.D
Acq On : 16 Jan 2023 10:42
Operator : CG/JU
Sample : PB150192BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150192BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.993	44.7	ng	6137660	1	7.905	2744700	20.0