


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
 Data File : BP013473.D
 Acq On : 16 Jan 2023 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 13 03:32:57 2023

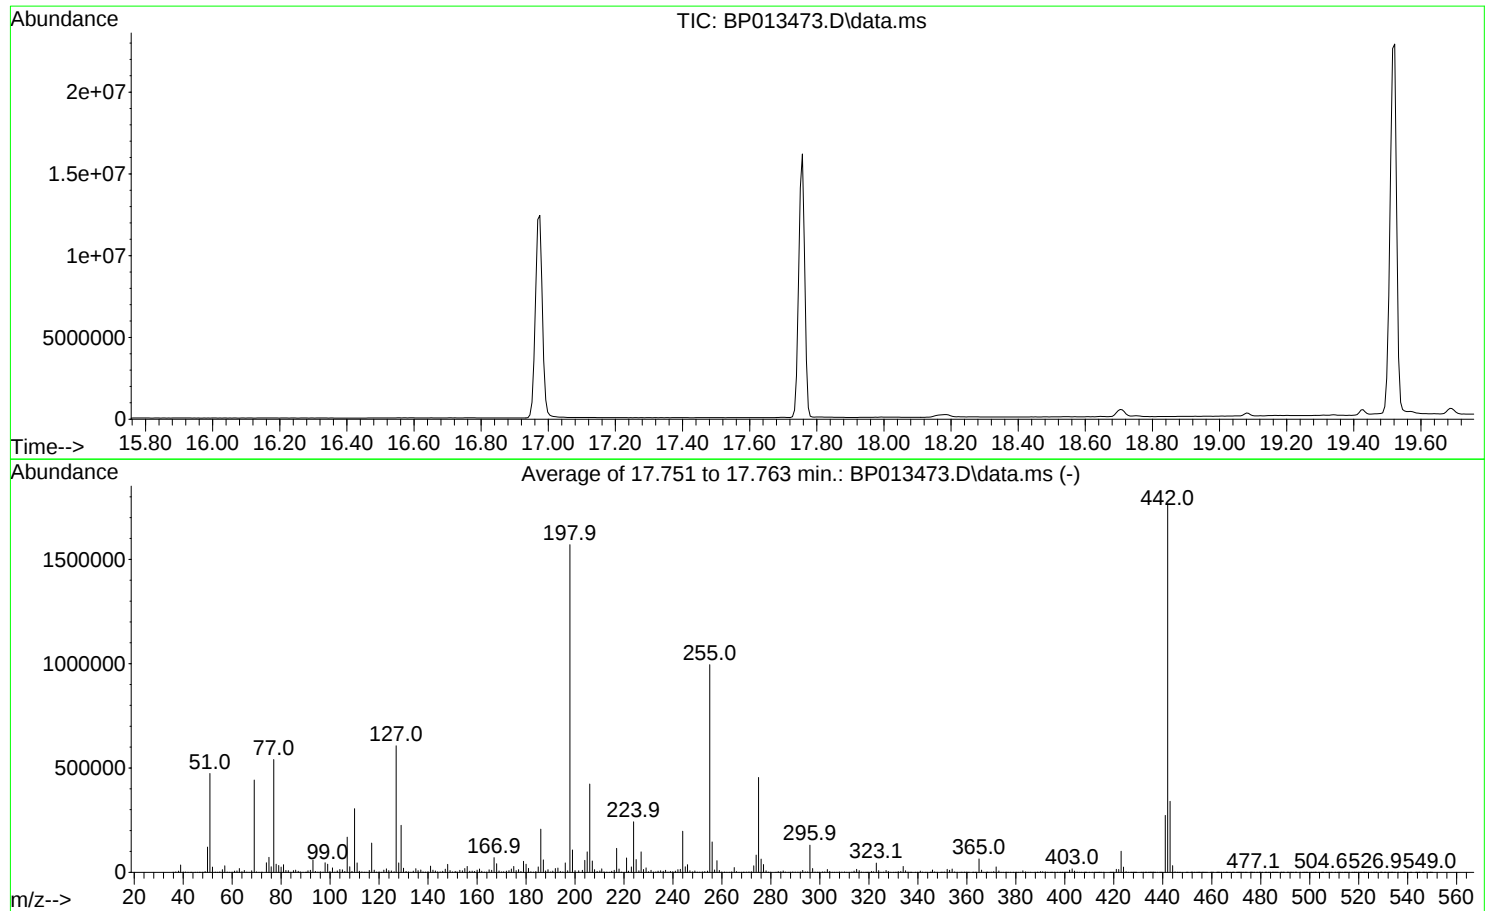




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	473488	PASS
68	69	0.00	2	1.7	7452	PASS
69	198	0.00	100	28.1	442081	PASS
70	69	0.00	2	0.5	2221	PASS
127	198	10	80	38.6	606425	PASS
197	198	0.00	2	0.5	7519	PASS
198	198	100	100	100.0	1570583	PASS
199	198	5	9	6.8	106929	PASS
275	198	10	60	28.9	454498	PASS
365	198	1	100	4.1	63749	PASS
441	198	0.01	100	17.3	272320	PASS
442	442	100	100	100.0	1763328	PASS
443	442	15	24	19.3	340474	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
Data File : BP013473.D
Acq On : 16 Jan 2023 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 17 07:36:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

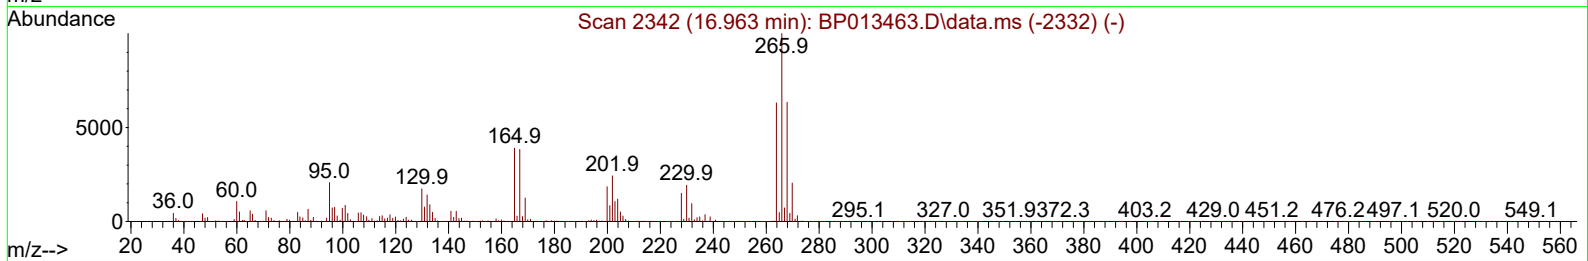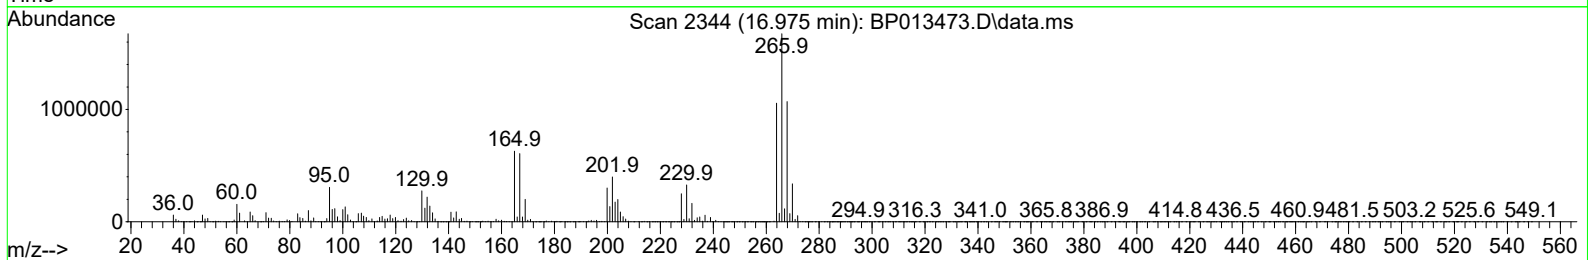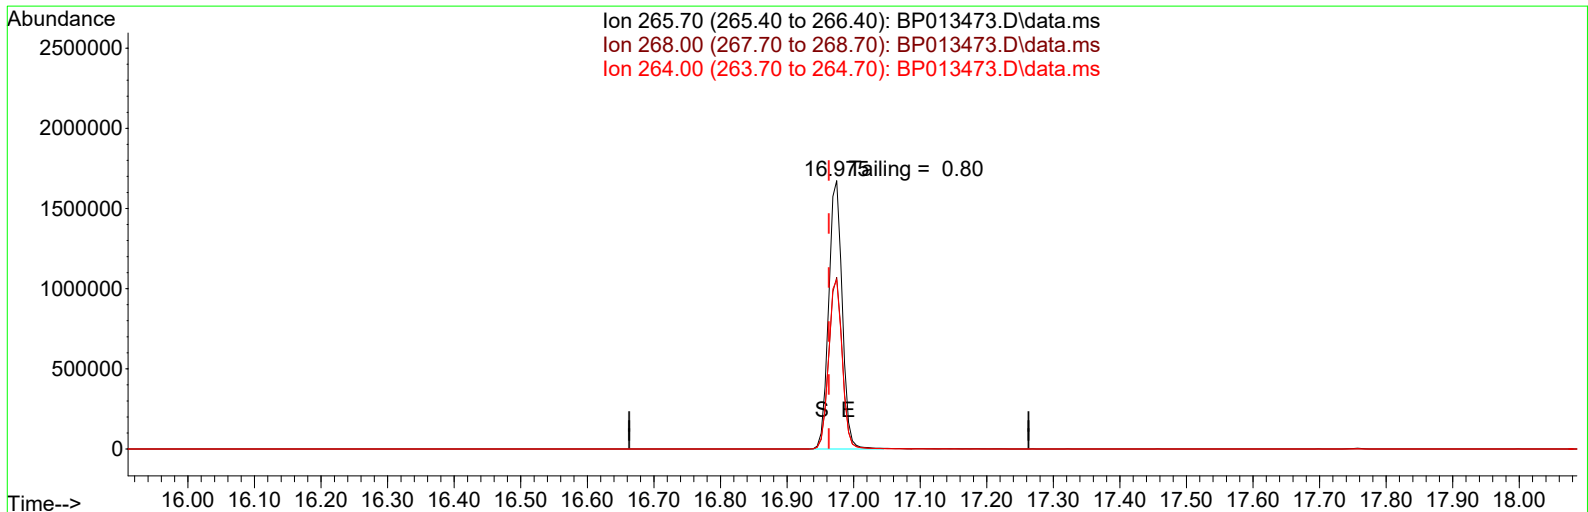

TIC: BP013473.D\data.ms

(70) Pentachlorophenol (C)

16.975min (+ 0.012) 1088747.58 ng




response 2380746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.93
264.00	63.00	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011623\
 Data File : BP013473.D
 Acq On : 16 Jan 2023 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 17 07:36:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 13 03:32:57 2023
 Response via : Initial Calibration

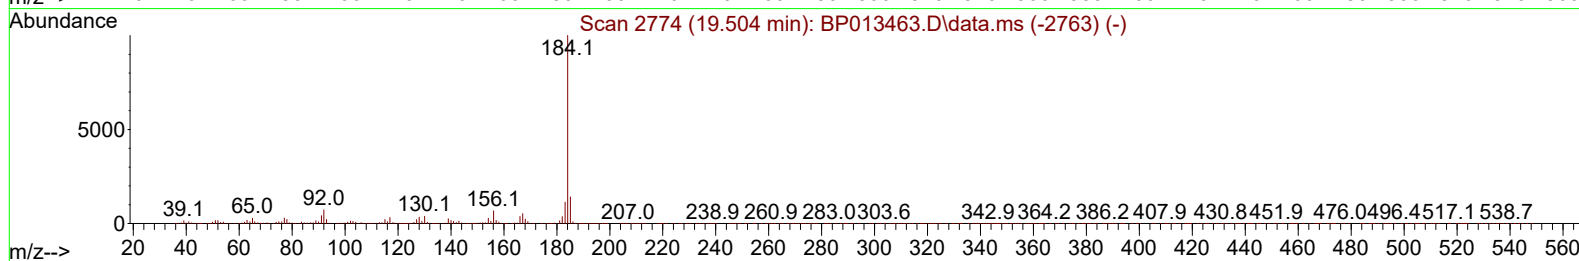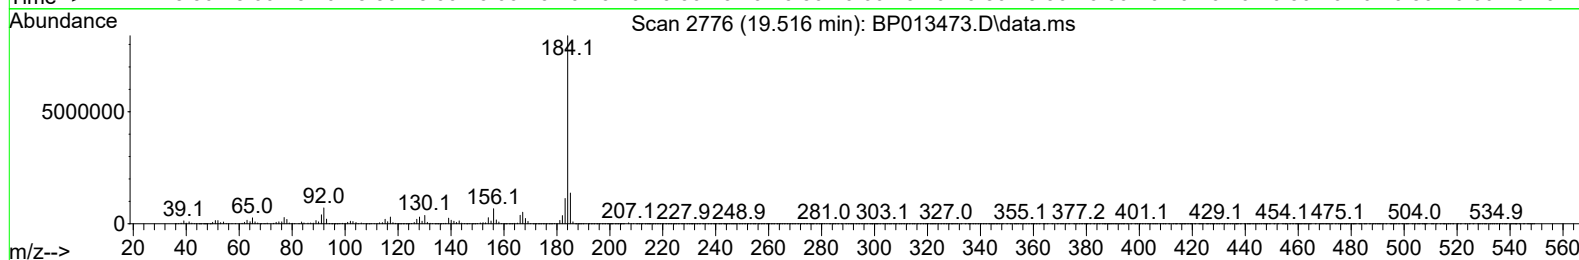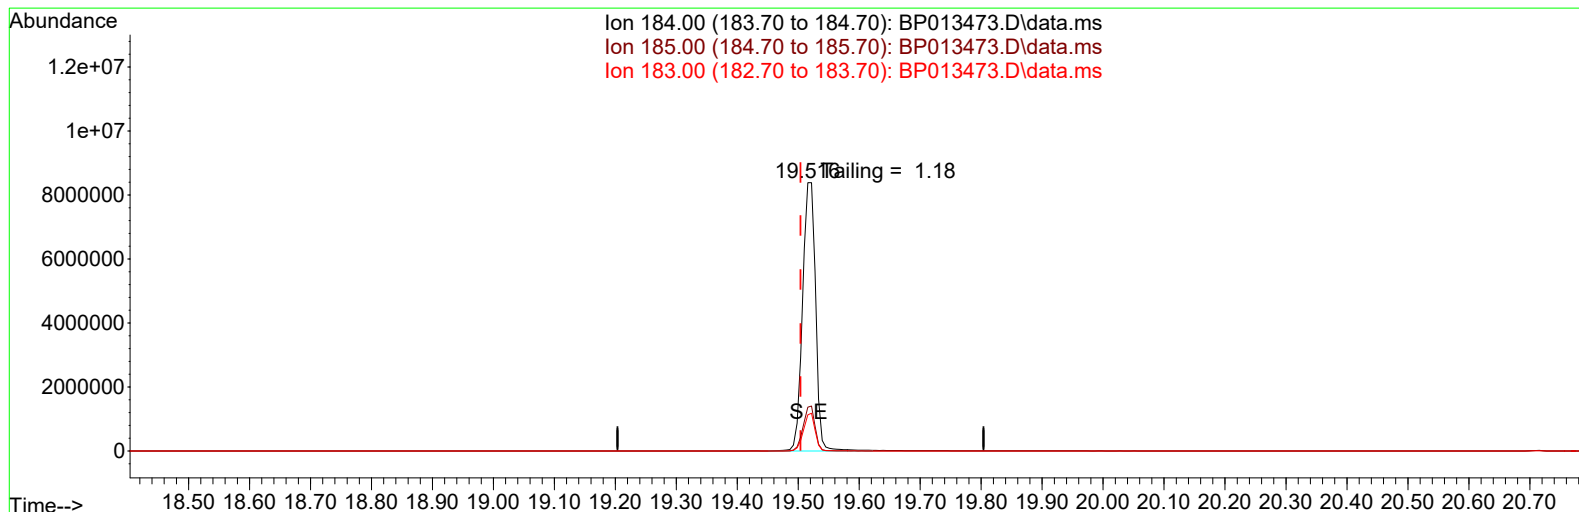

TIC: BP013473.D\data.ms

(77) Benzidine

19.516min (+ 0.012) 12243.37 ng m

response 12512879

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	16.35
183.00	11.40	13.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/16/2023	BNA_P	<u>BP013473.D</u>
Compound Name	Response	Retention Time
DDT	6075684	20.716
DDD	78117	20.333
DDE	9571	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
87688	6163372	1.42

Instrument :
BNA_P
ClientSampleId :
DFTPP