

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011624\
 Data File : BP019387.D
 Acq On : 16 Jan 2024 11:51
 Operator : MA/JU
 Sample : P1130-11DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2DL

Quant Time: Jan 16 12:23:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 03:05:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	129557	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.569	136	525366	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.416	164	376802	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.175	188	947747	20.000	ng/u1	-0.01
79) Chrysene-d12	21.280	240	962346	20.000	ng/u1	0.00
88) Perylene-d12	23.639	264	979943	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	6882	2.009	ng/uL	0.00
4) Pyridine-d5	3.640	84	47514	4.796	ng/u1	0.00
7) Phenol-d5	6.969	99	34000	2.746	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	123047	16.613	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.311	132	105716	12.428	ng/u1	0.00
15) 4-Methylphenol-d8	8.505	113	67358	6.857	ng/u1	-0.01
21) Nitrobenzene-d5	8.940	128	75826	17.156	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.663	143	84059	16.368	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	157279	15.159	ng/u1	0.00
31) 4-Chloroaniline-d4	10.722	131	143568	10.955	ng/u1	0.00
46) Dimethylphthalate-d6	13.840	166	588540	17.680	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	607425	17.022	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.687	143	12789	2.502	ng/u1	0.02
60) Fluorene-d10	15.416	176	511775	18.778	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	109182	15.604	ng/u1	0.00
73) Anthracene-d10	17.275	188	885951	18.743	ng/u1	-0.01
81) Pyrene-d10	19.522	212	1161674	18.512	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.486	264	1021526	19.171	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	65066	18.334	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011624\
Data File : BP019387.D
Acq On : 16 Jan 2024 11:51
Operator : MA/JU
Sample : P1130-11DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2DL

Quant Time: Jan 16 12:23:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 09 03:05:24 2024
Response via : Initial Calibration

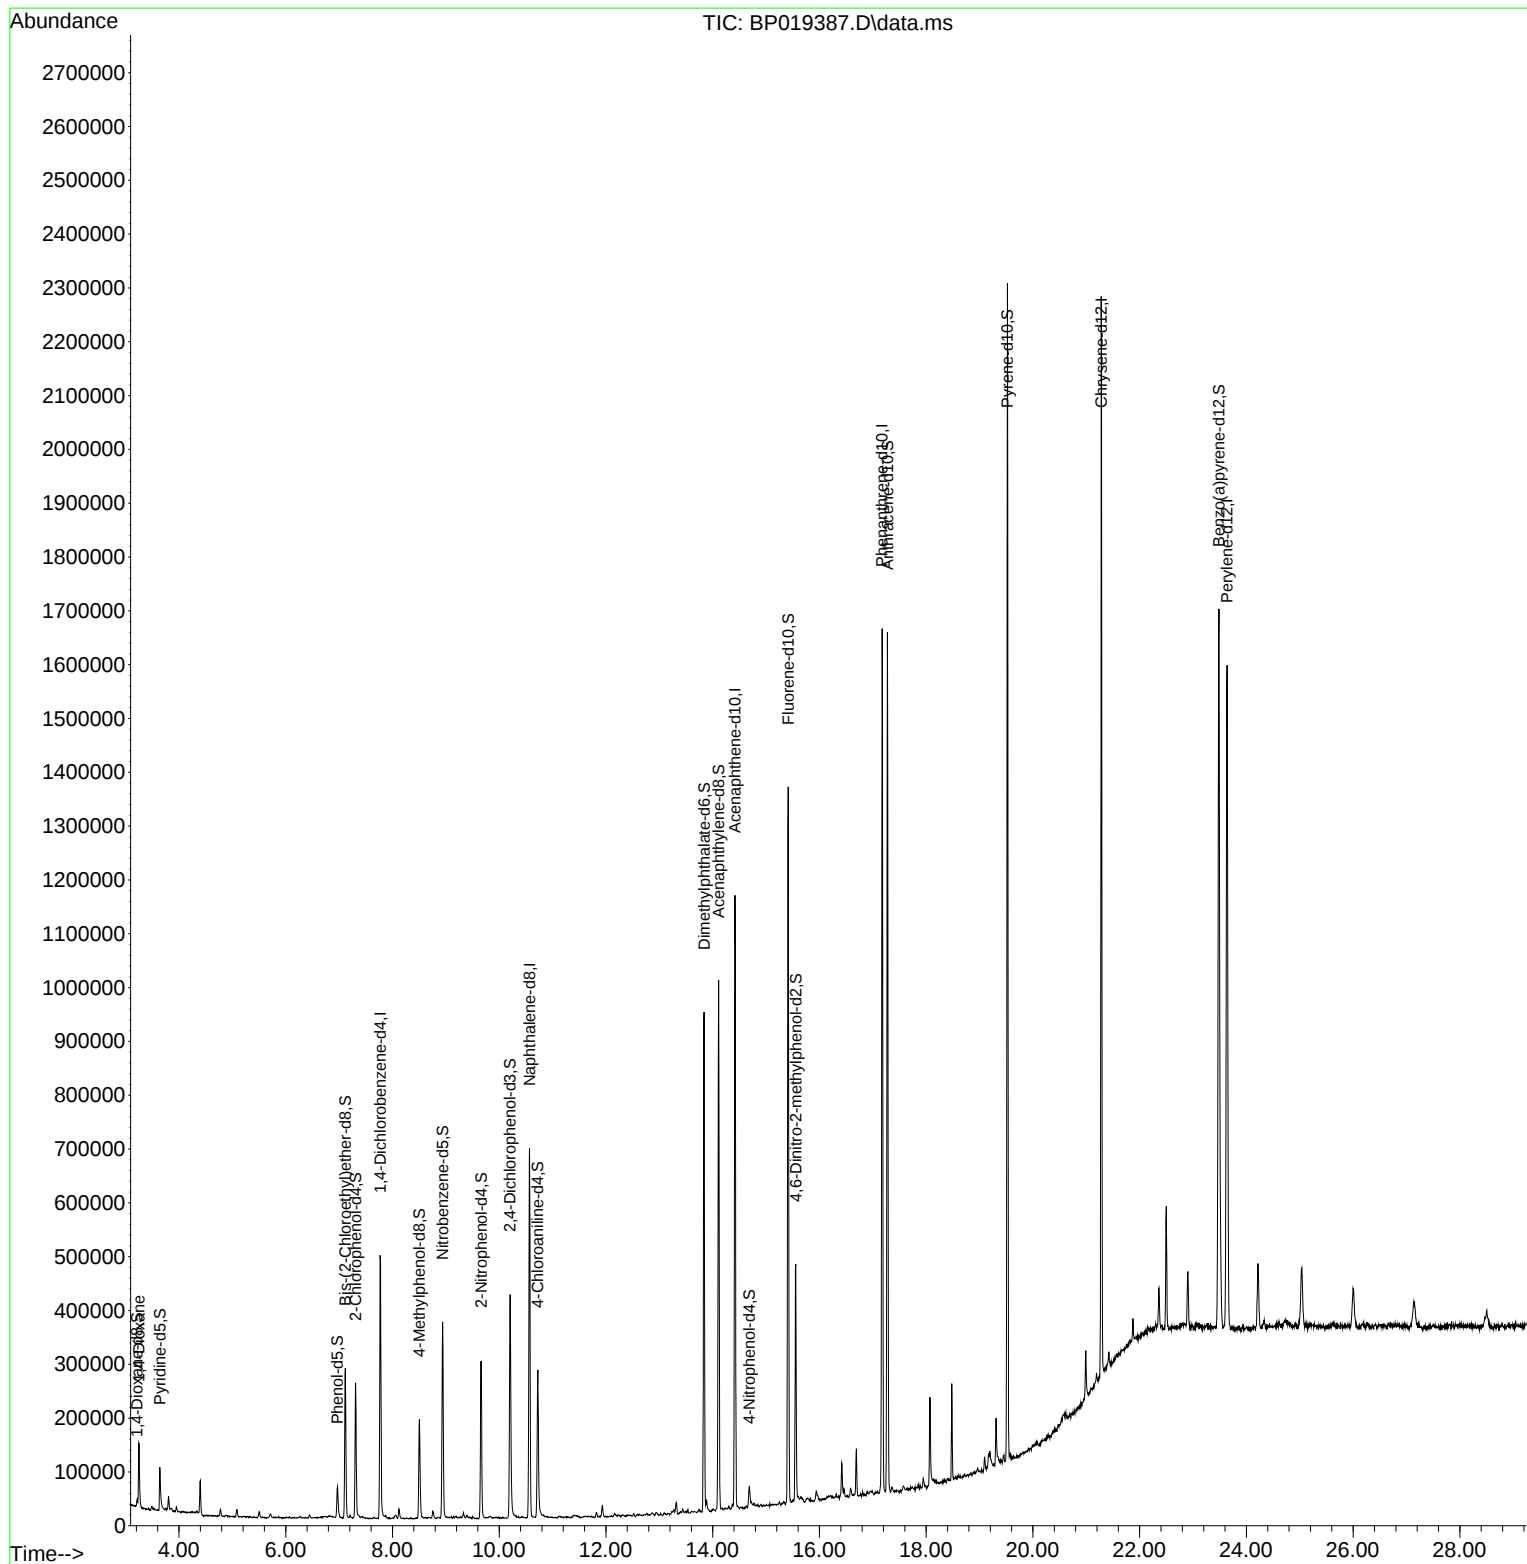

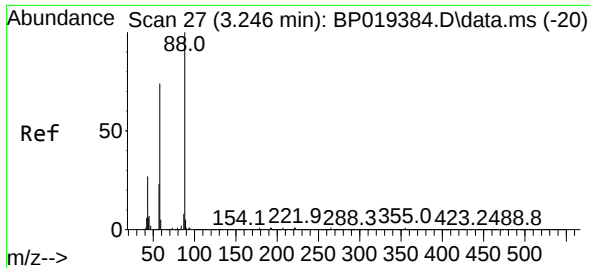

#2
 1,4-Dioxane
 Concen: 18.334 ng/uL
 RT: 3.252 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP019387.D
 Acq: 16 Jan 2024 11:51

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2DL

Tgt Ion: 88 Resp: 65066
 Ion Ratio Lower Upper
 88 100
 43 24.1 22.0 33.0
 58 65.7 54.6 82.0

