

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
 Data File : BP023614.D
 Acq On : 16 Jan 2025 11:39
 Operator : RC/JU
 Sample : Q1084-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BA2

Quant Time: Jan 16 12:14:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 16:27:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	402735	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	1636104	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	992686	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	1979311	20.000	ng/u1	-0.02
79) Chrysene-d12	21.692	240	1944451	20.000	ng/u1	-0.02
88) Perylene-d12	25.133	264	2169210	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	58594	5.364	ng/uL	0.00
4) Pyridine-d5	3.723	84	125428	4.119	ng/u1	0.00
7) Phenol-d5	6.963	99	248751	7.174	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	794923	39.136	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	846643	30.919	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	504418	18.756	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	470785	37.699	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	296550	36.179	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	820083	32.893	ng/u1	0.00
31) 4-Chloroaniline-d4	10.704	131	51686	1.299	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	2939601	38.050	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	3479964	37.865	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	48338	3.764	ng/u1	-0.01
60) Fluorene-d10	15.434	176	2657100	39.741	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	140966	21.889	ng/u1	-0.01
73) Anthracene-d10	17.328	188	4231621	39.605	ng/u1	-0.02
81) Pyrene-d10	19.704	212	4972075	46.157	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.904	264	5008311	42.485	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	15421	1.334	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023614.D
Acq On : 16 Jan 2025 11:39
Operator : RC/JU
Sample : Q1084-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA2


Quant Time: Jan 16 12:14:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 16:27:27 2025
Response via : Initial Calibration

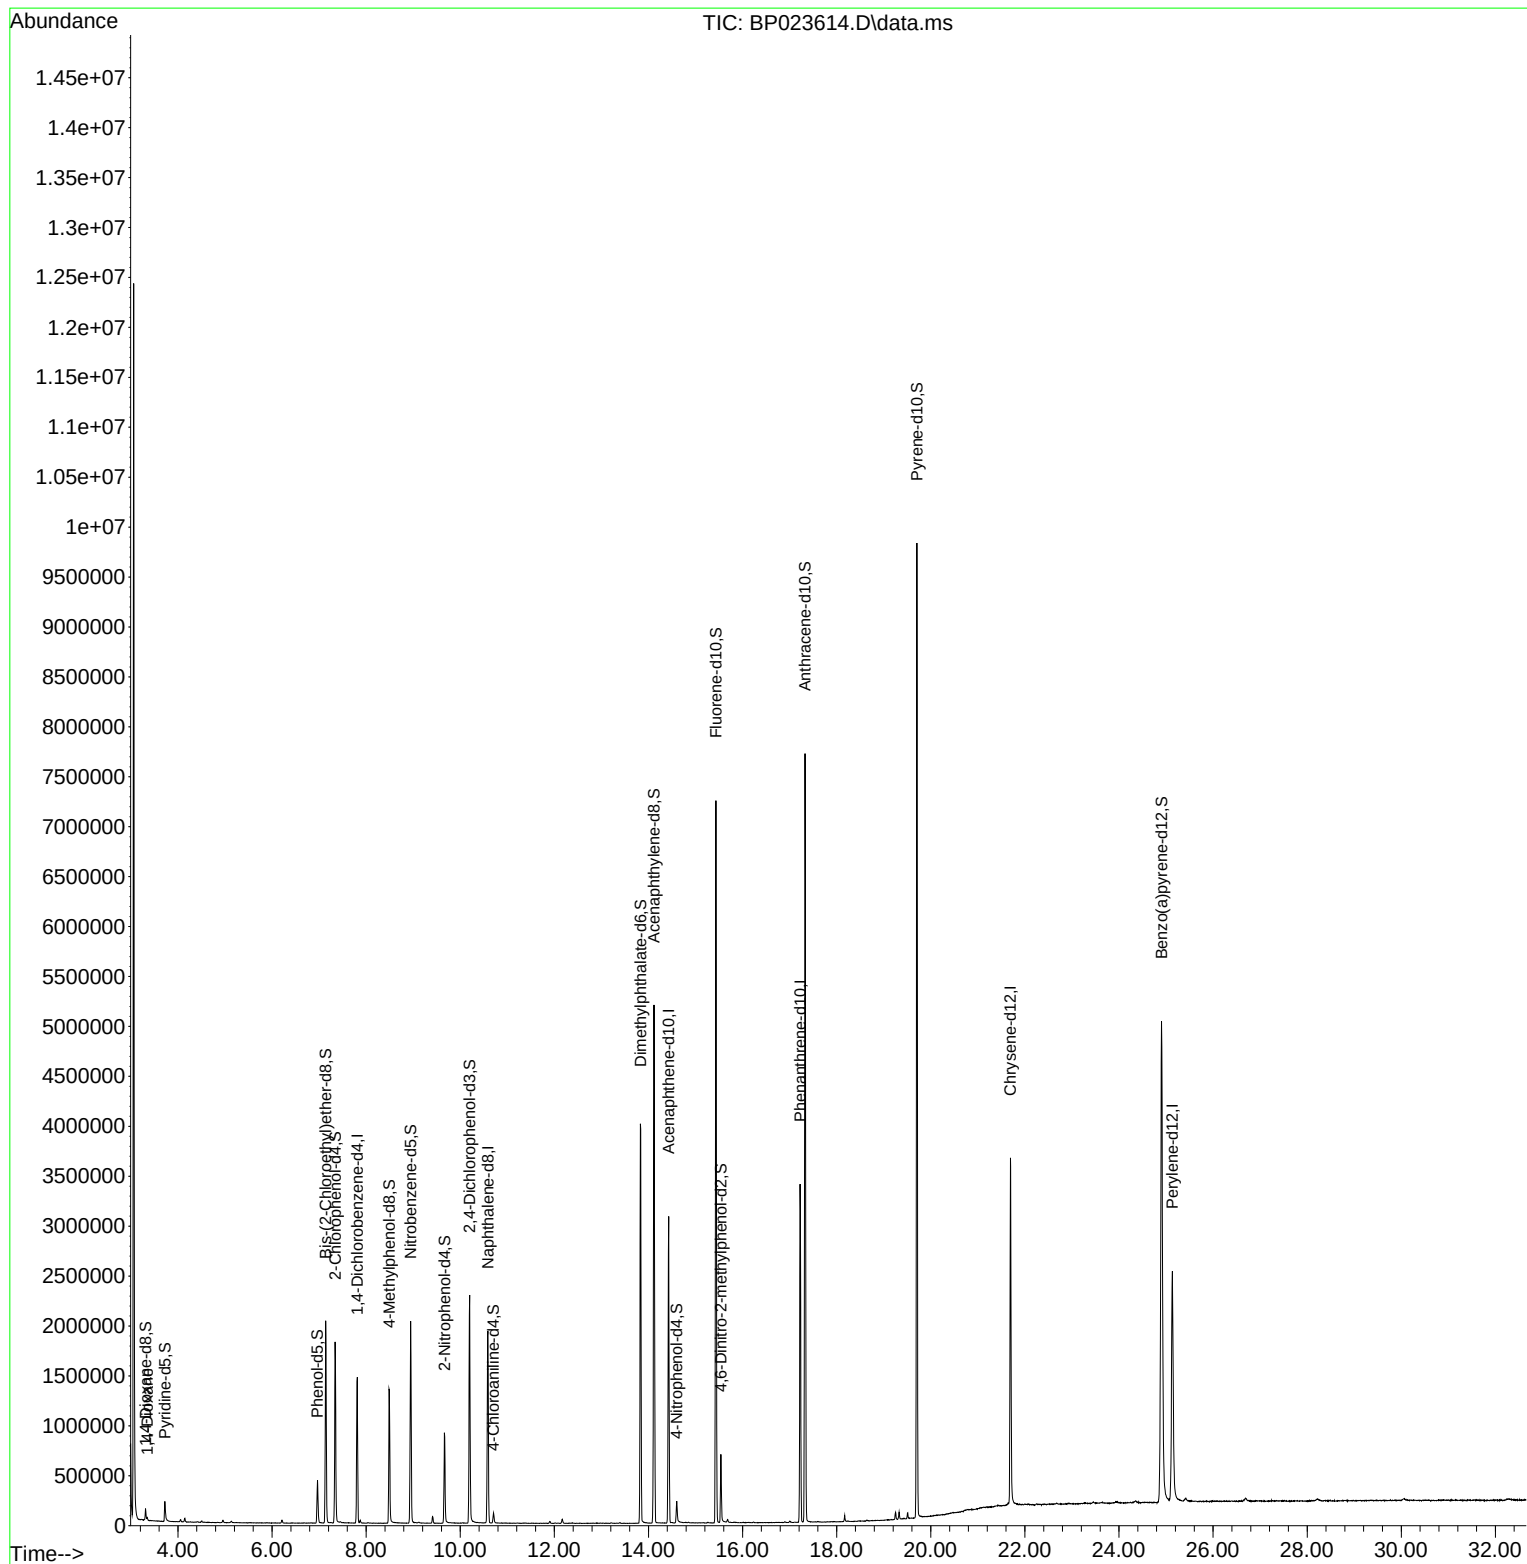

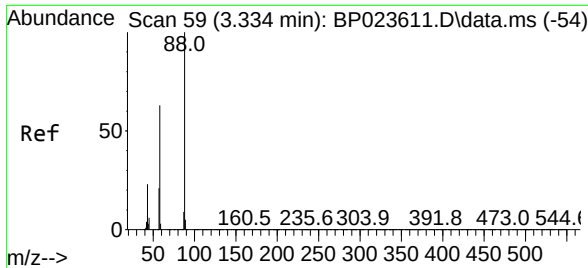

#2
 1,4-Dioxane
 Concen: 1.334 ng/uL
 RT: 3.346 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BP023614.D
 Acq: 16 Jan 2025 11:39

Instrument :
 BNA_P
 ClientSampleId :
 C0BA2

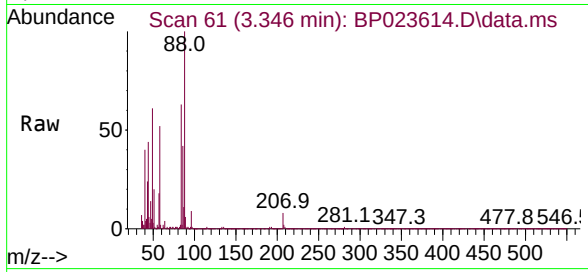

Tgt Ion: 88 Resp: 15421

Ion	Ratio	Lower	Upper
88	100		
43	23.6	17.3	25.9
58	52.2	47.4	71.0

