

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
 Data File : BP023615.D
 Acq On : 16 Jan 2025 12:20
 Operator : RC/JU
 Sample : Q1084-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BA4

Quant Time: Jan 16 12:52:52 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 16:27:27 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	328630	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	1397211	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	880615	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	1810138	20.000	ng/u1	0.00
79) Chrysene-d12	21.698	240	1834180	20.000	ng/u1	-0.01
88) Perylene-d12	25.127	264	2003450	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	48552	5.447	ng/uL	0.00
4) Pyridine-d5	3.723	84	80486	3.239	ng/u1	0.00
7) Phenol-d5	6.964	99	184172	6.509	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	650186	39.229	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	661901	29.623	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	382868	17.446	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	383186	35.931	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	233682	33.383	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	648913	30.477	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	492147	14.479	ng/u1	0.00
46) Dimethylphthalate-d6	13.840	166	2714322	39.605	ng/u1	0.00
49) Acenaphthylene-d8	14.122	160	3014856	36.979	ng/u1	0.00
54) 4-Nitrophenol-d4	14.616	143	41337	3.629	ng/u1	0.00
60) Fluorene-d10	15.445	176	2463674	41.537	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	136952	23.253	ng/u1	0.00
73) Anthracene-d10	17.345	188	4155723	42.530	ng/u1	0.00
81) Pyrene-d10	19.716	212	5022658	49.430	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.904	264	5088063	46.732	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.346	88	13700	1.453	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023615.D
Acq On : 16 Jan 2025 12:20
Operator : RC/JU
Sample : Q1084-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA4


Quant Time: Jan 16 12:52:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 16:27:27 2025
Response via : Initial Calibration

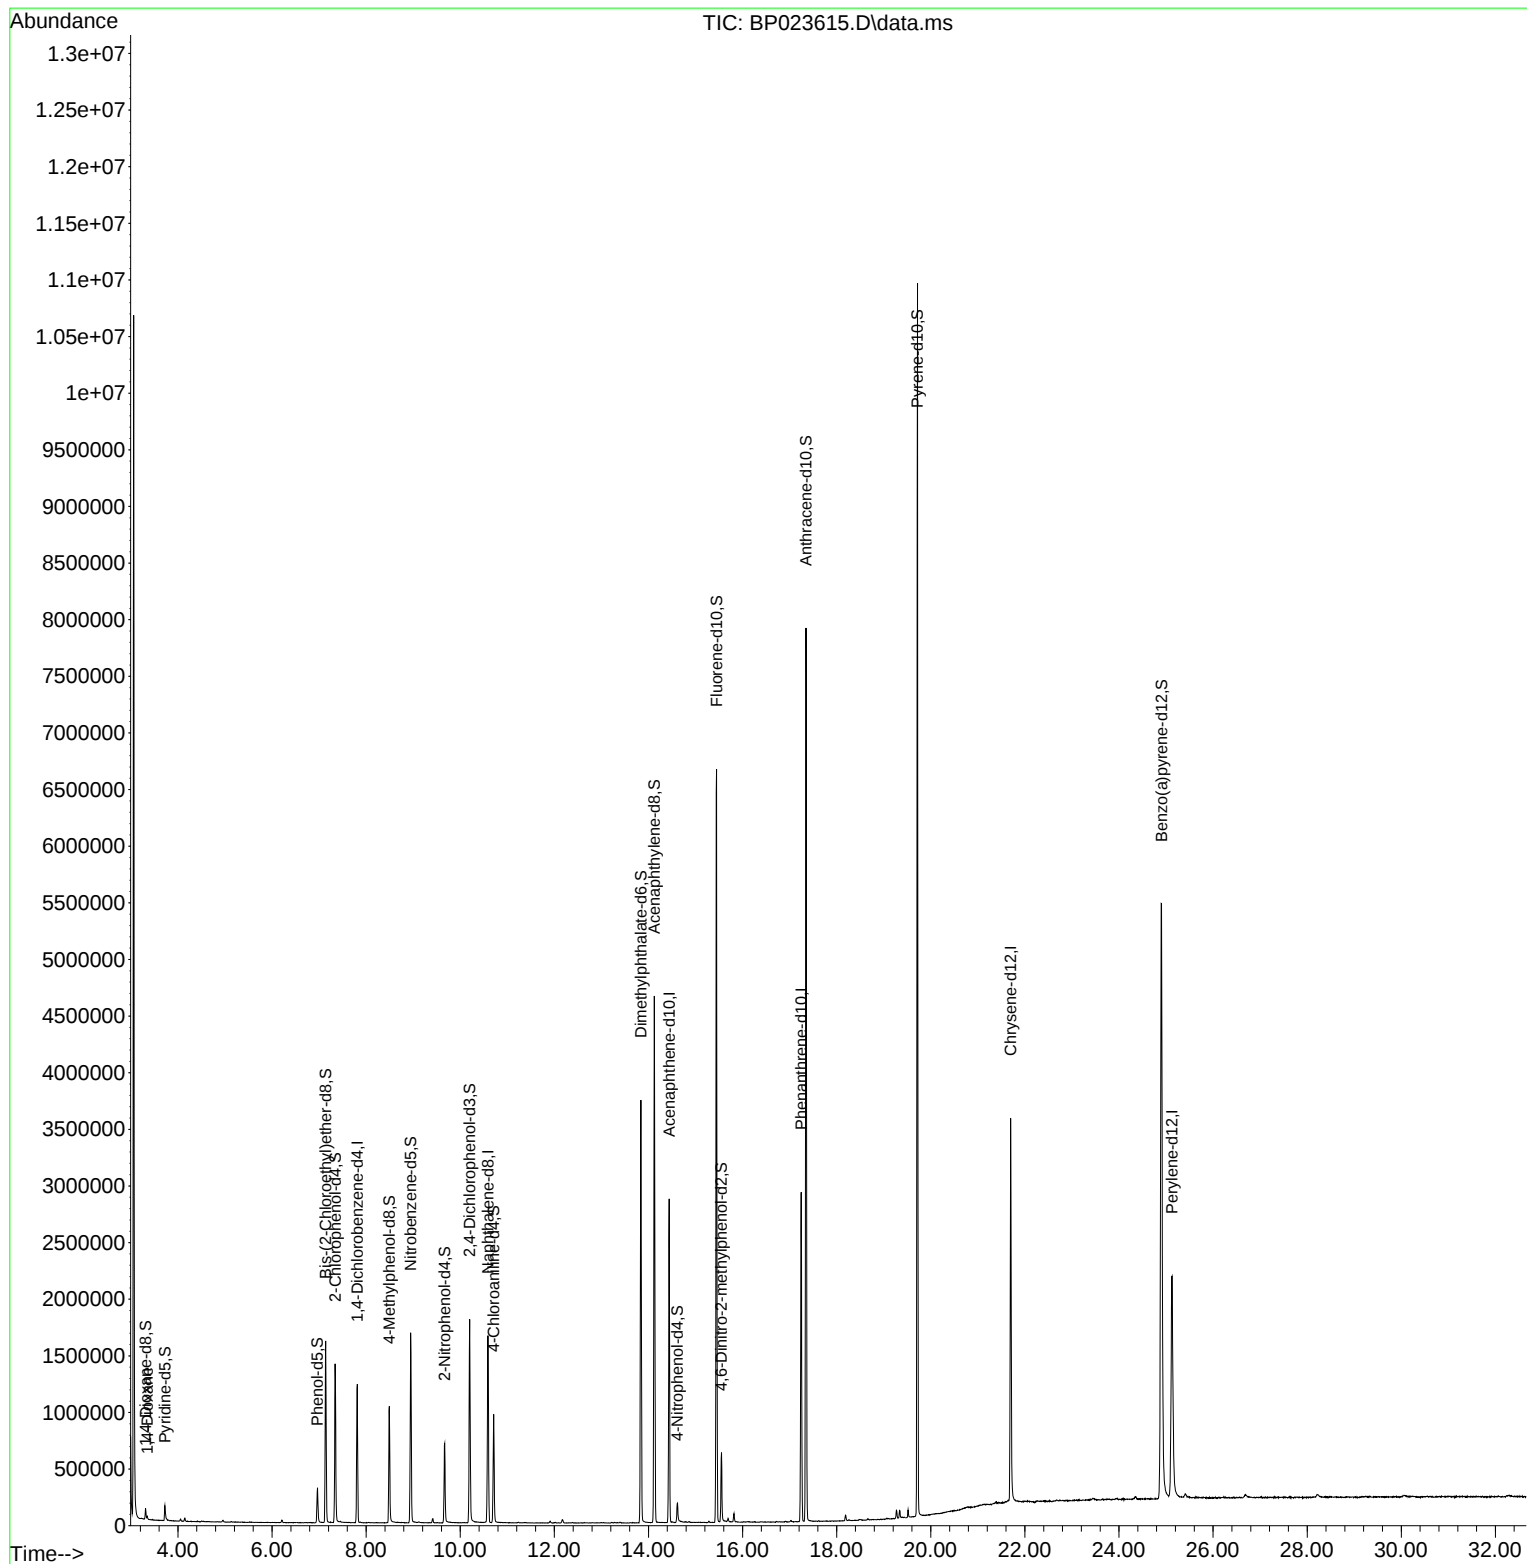

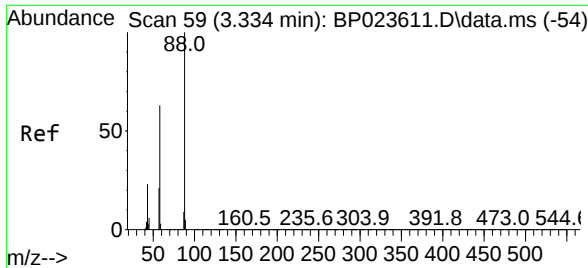

#2
 1,4-Dioxane
 Concen: 1.453 ng/uL
 RT: 3.346 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BP023615.D
 Acq: 16 Jan 2025 12:20

Instrument :
 BNA_P
 ClientSampleId :
 C0BA4

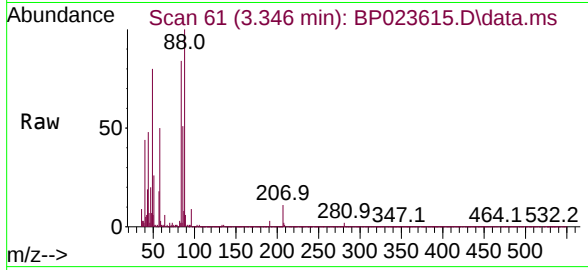

Tgt Ion:	88	Resp:	13700
Ion	Ratio	Lower	Upper
88	100		
43	18.8	17.3	25.9
58	50.2	47.4	71.0

